

APPLIED KILOVOLTS

SHPZ

Oct 07

SAFETY & INSTALLATION INSTRUCTIONS FOR HPZ SERIES

PLEASE READ CAREFULLY BEFORE INSTALLING OR OPERATING THIS POWER SUPPLY


Power Supply Warning Symbols


Caution,
Risk of electric shock



Caution
Refer to accompanying documentation



HV Output  connect screen (shield) of cable to system ground (earth)

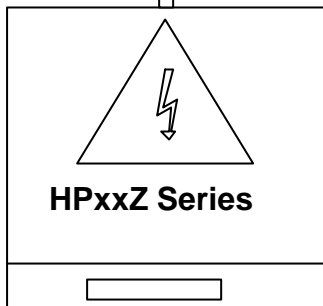

Internal manual
potentiometer not fitted

Note 1

AA= Option Code:

IP = Standard unit = Precision Imonitor

OP= Polarity Option¹ (+Precision Imonitor)

e.g. Order Code:

HP003ZIP025 ±3kV 400µA standard unit

HP010ROP025 ±10kV 400µA + Polarity Option¹

Polarity Option – height increases to 52mm:

Pin 8 Control input becomes 0V to +10V only.

Pin 18 becomes Polarity Input H= Pos

Pin 20 becomes INH input H= ON

PIN CONNECTIONS

Input Connector: BERG 20 Way IDC header Part No 65863-069 for use with ribbon cable.

1	+24V Power supply input ²	11	Power ground ²
2	nc	12	Power ground ²
3	+24V Power supply input ²	13	Power ground ²
4	V Monitor	14	Signal ground
5	+24V Power supply input ²	15	Power ground ²
6	I Monitor	16	nc
7	+24V Power supply input ²	17	Power ground ²
8	-10V to +10V Control input ¹	18	nc ¹ Polarity i/p
9	24V Power supply input	19	Power ground
10	Control input return	20	nc ¹ Inhibit

Note 2. The input connector pins are not rated at the full input current of the power supply.

Please use at least 2 pins in parallel for the +24V power supply input & the power ground.

For mating Connector & 300mm of ribbon cable - order part no ID20

SPECIFICATION

UNIT	OUTPUT	RIPPLE	SIZE (mm)
HP001ZIP025	-1 kV to +1 kV at 1mA	55 mV peak to peak	162 x 184 x 47 mm ¹
HP2.5ZIP025	-2.5 kV to +2.5 kV at 400uA	70 mV peak to peak	162 x 184 x 47 mm ¹
HP003ZIP025	-3 kV to +3 kV at 400uA	75 mV peak to peak	162 x 184 x 47 mm ¹
HP005ZIP025	-5 kV to +5 kV at 400uA	170 mV peak to peak	162 x 184 x 47 mm ¹
HP008ZIP025	-8 kV to +8 kV at 400uA	300 mV peak to peak	162 x 184 x 47 mm ¹
HP010ZIP025	-10 kV to +10 kV at 400uA	300 mV peak to peak	162 x 184 x 47 mm ¹

Input Supply Voltage 24Vdc ± 10% at 1A .

Mounting By 4 off M3 blind fasteners.

Cover M3 screws – maximum length 6mm

Cleaning Use a lint free cloth soaked with isopropyl alcohol, ensuring the unit is completely dry before use.

Environmental Conditions

Indoor use only,

Operating Temperature 0°C to +45°C,

Altitude up to 2000m,

Storage Temperature -35°C to +85°C.

Maximum relative humidity 80% for temperatures up to 31°C, decreasing linearly to 50% relative humidity at 40° C,

The unit is to be supplied from a current limited supply providing 24Vdc, impulse limited to (overvoltage) Category I of IEC60364-4-443.

For use in an environment of pollution degree 2.

Applied Kilovolts Ltd., Woods Way, Goring by Sea, West Sussex BN12 4QY, UK.

Tel: +44 (0) 1903 708850 Fax +44 (0) 1903 708851

GENERAL

On receipt the unit should be carefully unpacked and inspected to ensure that no transit damage has occurred. Provided that this inspection is satisfactory and reveals no evidence of damage then installation can proceed.

If an electrical test is to be carried out prior to fitting the power supply, it is essential that the person undertaking this work has received appropriate technical training to be aware of the hazards to which that person may be exposed in performing the tests, and of measures to minimise the risks to themselves, and other personnel. Metallic or conductive tools should not be used to adjust any of the potentiometers. The unit has no user serviceable parts and should not be dismantled.

DO NOT HANDLE OR TOUCH THESE UNITS WHEN THE SUPPLY IS CONNECTED. AFTER DISCONNECTION FROM THE SUPPLY, ALLOW 30 SECONDS BEFORE HANDLING SO THAT ALL THE CAPACITORS CAN DISCHARGE. To ensure that the output is fully discharged short to ground before touching any high voltage circuit.

Care should be taken not to operate the unit outside the specified limits given above. Failure to do so may damage the unit.

COMPLIANCE WITH SAFETY STANDARDS

The unit is designed to meet Normalised European Safety Standards for installation in equipment conforming to EN61010 and hence installation of the power supply unit into the equipment should comply with the following requirements.

- a. A PROTECTIVE EARTH must be provided for safety in accordance with EN61010 Part 1 : Clause 6.5.1. The case of the units should be bonded to this protective earth.
- b. The output is classed as hazardous and must therefore not be accessible to operators. The output must be isolated from accessible circuits by Double Insulation or a protective screen as defined in EN61010-1.
- c. It is intended to be installed in an electrical enclosure and the unit and its input connector should not be accessible to the operator. Access should be restricted to authorised service personnel only, with use of a tool. Care should be taken to prevent access to the interior of the unit and protect against items (e.g. tools or wires) inadvertently entering the interior of the unit.
- d. The unit is not fitted with a fuse and so should be operated from a limited supply of <2 amp.

INSTALLATION

The outputs of these units are considered hazardous and should be installed such that they cannot become accessible. The output should be connected such that the shortest creepage and clearance path is to a protective earth connection. ENSURE that a LOW IMPEDANCE connection is made to the unit chassis from the system PROTECTIVE EARTH. The safety earth conductor must not contain any switches or fuses.

Under worst case conditions the unit draws a current of 1.3A and any input supply cable must be of a suitable type and rating. The unit is not fitted with a fuse and so should be operated from a limited supply. Fuses may be fitted externally to the unit to protect unit and interconnecting wiring etc. but these should be rated to prevent nuisance failures. Care should be taken in the design of the interconnecting wiring within the system to ensure that connectors with hazardous voltages cannot be connected to accessible circuits.

Ensure that the output is connected to the load prior to operation of the unit and that a good low impedance high voltage joint is made. Sharp points on either the high voltage or return joint should be avoided as this will cause corona which will make the output appear noisy. In general a tracking distance (creepage distance) of 25mm (1 inch), per 10kV to earth is advised as a minimum to ensure no breakdown or corona occurs, a much greater distance will be required under adverse conditions. Care must be taken not to damage the cable inner when forming the connections.

During arcing currents exceeding 1000 Amps will flow. It is important that these currents return to the high voltage power supply by the shortest possible route using the screen of the output cable. Failure to observe this will result in the control terminals of the unit seeing large voltage spikes during arcing and radiation of electromagnetic interference.

Adequate ventilation should be provided to keep the unit cool and the ventilation inlets should not be covered in any way. The ambient air temperature around the inlet must not exceed 45°C. The unit will operate in any orientation, however it is not recommended to operate with the side fitted with the silk-screen as the lowest face.

OPERATING NOTES

- 1/ HIGH VOLTAGES ARE DANGEROUS. ENSURE THE OUTPUT IS FULLY DISCHARGED BY SHORTING TO GROUND BEFORE TOUCHING ANY HIGH VOLTAGE CIRCUIT.
- 2/ The unit is short circuit proof but care should be taken that the high voltage cannot be shorted into one of the control pin connections.