




1. 底部のゴム足、側面のゴム足およびハンドルを取り外します。



機器が落下する恐れがあります。
使用するラックに適合したサポートアングルを
取り付けて、本体を支持してください。




No.	コード	説 明	数量
1	B9-000-026	BRKT KRB150-TOS L/R	2
2	B9-000-044	BRKT KRB150-PLZ-50F TOP	1
3	M2-101-015	FLH SCREW S-NI M4X0.7X8	6
4	M2-102-002	OVH SCREW S-NI M5X0.8X14	4
5	M5-003-031	CUP WASHER 5 CW	4

INSTRUCTION MANUAL


Bracket KRB150-PLZ-50F

Install the brackets to the instrument in the next procedure and build in it to the rack.


1. Remove the rubber feet on the bottom panel, the rubber feet on the side panel and handle.

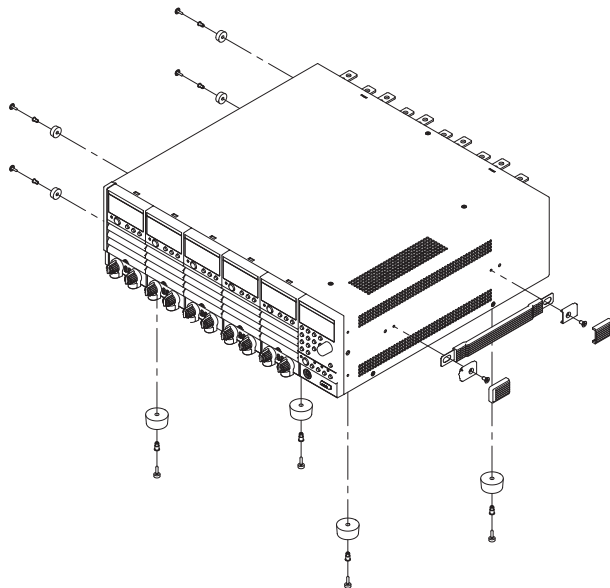


2. As shown in figure, using (3) screws, install (1) and (2) brackets.
For (3) screws, do not use except the accompanying screws (M4 x 8 flat head screws).

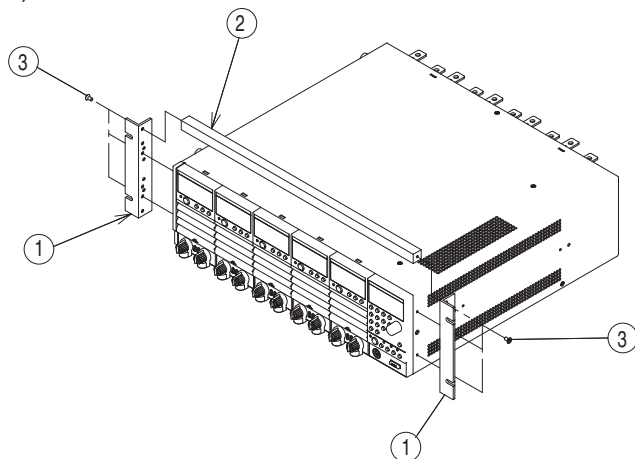

3. Using (4) screws and (5) washers, mount the instrument in the rack.

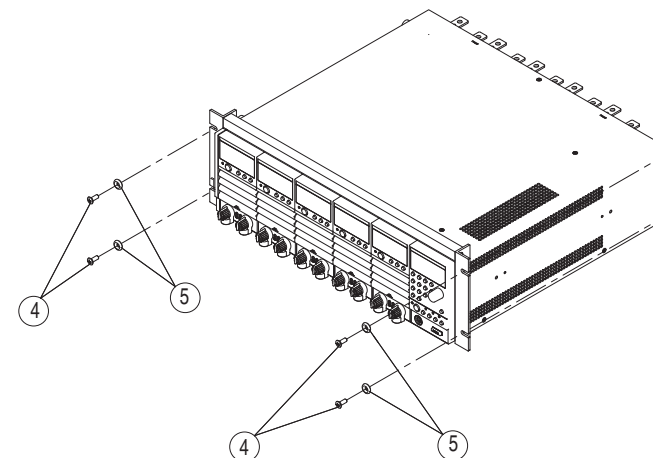

CAUTION The instrument may fall.
Install the suitable support angles
applying to the used rack system to
support the instrument.



No.	CODE	DESCRIPTION	QTY
1	B9-000-026	BRKT KRB150-TOS L/R	2
2	B9-000-044	BRKT KRB150-PLZ-50F TOP	1
3	M2-101-015	FLH SCREW S-NI M4X0.7X8	6
4	M2-102-002	OVH SCREW S-NI M5X0.8X14	4
5	M5-003-031	CUP WASHER 5 CW	4



KIKUSUI ELECTRONICS CORP.

1-1-3, Higashiyamata, Tsuzuki-ku, Yokohama, 244-0023, Japan