



ブラケット KRB6-PAM

次の手順で機器にブラケットを取り付け、ラックに組み込みます。


1. 底部のゴム足を取り外します。

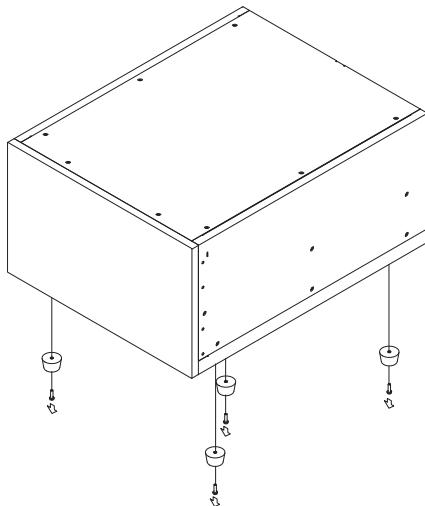


2. 付属のねじを使用してブラケットを図のように取り付けます。
付属のねじ(M4 x 10皿ねじ)以外は使用しないでください。

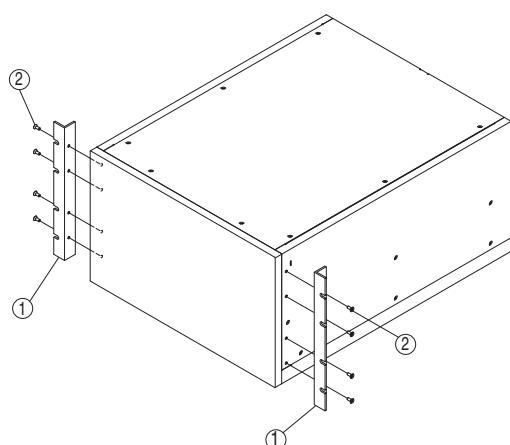

3. 付属のねじとワッシャを使用してラックに取り付けます。

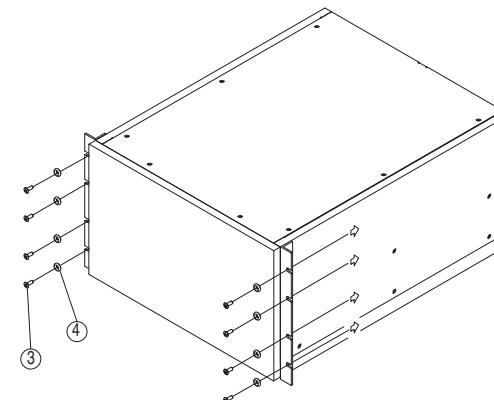

△ 注意 機器が落下する恐れがあります。
使用するラックに適合したサポートアングルを取り付けて、本体を支持してください。



No.	コード	説明	数量
1	B9-000-028	BRKT KRB6-PAM L/R	2
2	M2-001-161	SARA SCREW M4X0.7X10	8
3	M2-102-002	OVH SCREW S-NI M5X0.8X14	8
4	M5-003-031	CUP WASHER 5 CW	8

Part No. Z1-901-180, IA002733

 KIKUSUI


菊水電子工業株式会社

本社・技術センター 〒224-0023 横浜市都筑区東山田 1-1-3 TEL: 045-593-0200 (代)


BRACKET KRB6-PAM

Install the brackets to the instrument in the next procedure and build in it to the rack.


1. Remove the rubber feet on the bottom panel.

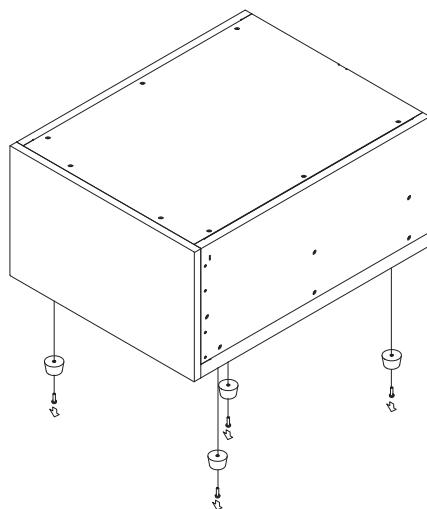


2. As shown in figure, using the accompanying screws, install the brackets. Do not use except the accompanying screws (M4 x 10 flat head screws).

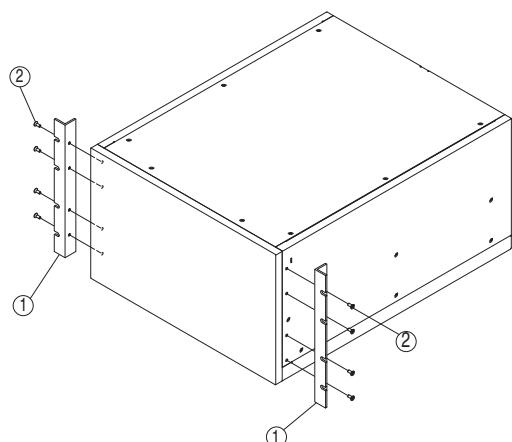

3. Using the accompanying screws and washers, mount the instrument in the rack.

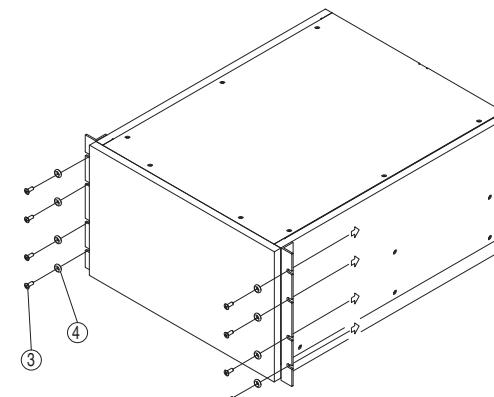

CAUTION The instrument may fall. Install the suitable support angles applying to the used rack system to support the instrument.



No.	CODE	DESCRIPTION	QTY
1	B9-000-028	BRKT KRB6-PAM L/R	2
2	M2-101-016	FLH SCREW S-NI M4X0.7X10	8
3	M2-102-002	OVH SCREW S-NI M5X0.8X14	8
4	M5-003-031	CUP WASHER 5 CW	8



KIKUSUI ELECTRONICS CORP.

1-1-3, Higashiyamata, Tsuzuki-ku, Yokohama, 244-0023, Japan