INSTRUCTION MANUAL

REMOTE CONTROLLERS

MODELS RC01-AVM & RC02-AVM

Power Requirements of this Product

| Power requirements of this product have been changed and the relevant sections of the Operation Manual should be revised accordingly. (Revision should be applied to items indicated by a check mark .) |
|---|
| ☐ Input voltage |
| The input voltage of this product is VAC, and the voltage range is to VAC. Use the product within this range only. |
| ☐ Input fuse |
| The rating of this product's input fuse isA,VAC, and |
| WARNING |
| To avoid electrical shock, always disconnect the AC power cable or turn off the switch on the switchboard before attempting to check or replace the fuse. |
| Use a fuse element having a shape, rating, and characteristics suitable for this product. The use of a fuse with a different rating or one that short circuits the fuse holder may result in fire, electric shock, or irreparable damage. |
| ☐ AC power cable |
| The product is porvided with AC power cables described below. If the cable has no power plug, attach a power plug or crimp-style terminals to the cable in accordance with the wire colors specified in the drawing. |
| The attachment of a power plug or crimp-style terminals |
| must be carried out by qualified personnel. |
| ☐ Without a power plug ☐ Without a power plug |
| Blue (NEUTRAL) White (NEUTRAL) |
| Brown (LIVE) Black (LIVE) |
| Green/Yellow (GND) Green or Green/Yellow (GND) |
| ☐ Plugs for USA ☐ Plugs for Europe |
| |
| |
| |
| Provided by Kikusui agents |
| Kikusui agents can provide you with suitable AC power cable. For further information, contact your Kikusui agent. |
| |
| Apother Cable |



TABLE OF CONTENTS

| | PAGE |
|--|------|
| 1. GENERAL | 1 |
| 2. SPECIFICATIONS | 2 |
| 3. GENERAL PRECAUTIONS | 4 |
| 3.1 Unpacking | 4 |
| 3.2 Power Source | 4 |
| 3.3 Environmental Conditions | 4 |
| 3.4 Others | 4 |
| 4. OPERATION METHOD | 5 |
| 4.1 Explanation of Panel Items | 5 |
| 4.2 Operation Method | 8 |
| 4.3 Programming Procedure | 8 |
| 4.3.1 Explanation of Programming Chart | 8 |
| 4.3.2 Example of Programming | 10 |
| 4.4 Notes for Noise and Longevity | 12. |

1. GENERAL

Remote Controller RCO1-AVM or RCO2-AVM is used in conjunction with AC Voltmeter AVM23R or AVM25R for range selection in 2-channel measurement, or with Programmable Oscillator ORC2l for programmed remote control of frequency address selection and on/off switching of R/L output signals.

Program setting can be made for up to 8 steps. For each step, a 16-position rotary-type code switch is used and programming can be done simply by using a screwdriver. The RCO1-AVM is a 2-channel type and RCO2-AVM is a 4-channel type, and programming can be done independently for each channel.

For switching operation, 8-linked-key push switches of soft touch and excellent longevity are used. Since programming can be made on two mutually independent grounds, the performance of AVM23R or other measuring instruments which have two mutually independent input channels can be made full use of.

Facilitating the installation work, the remote control cable can be run through the right, left, or rear side of the instrument case. The case can be mounted on an operation bench or other object by means of the threaded stud holes at the bottom of the case.

2. SPECIFICATIONS

2.1 Name of Instrument:

Remote Controller

2.2 Model No. of Instrument:

RCO1-AVM [RCO2-AVM]

2.3 Switching Operation

2.3.1 Step Selection System:

Push switch type (8-linked-key type,

2 circuits, 2 mutually independent

channels)

. 2.3.2 Programming System:

16-position rotary-type code switches

(internal setting).

2 steps per channel, 1 set per channel.

[4 channels per step, 1 set per channel]

2.3.3 Output Data Code:

Positive logic (4-bit binary for each

channel)

2.4 Selected Step Indicator

Red LED lamps. (The one selected

Lamps:

turns on.)

2.5 PANEL/REMOTE selector switch:

Slide switch

2.6 REMOTE Indication:

Indicated at the controlled equipment,

2.7 Remote Control Cable
 with Plug:

An approximately 2-m-long (6.6-ft long) remote control cable, with a nlug (Amphenol 57-Series 56-50240 plug at

the cable end),

2.8 Power Supplies and GND Terminals

2 channels

+5V1, GND1: Operation voltage 4 - 5 V,

current consumption 10 mA or less

+5V2. GND2: 0

Operation voltage 4 - 5 V.

current consumption 10 mA or less

(Supplied from the equipment controlled.)

+5V1, GND1:

1st row (REMOTE 1) code switches, and

digital IC power supply and GND

2nd row (REMOTE 2) code switches +5V1, GND1: 1st row (REMOTE 1) and 3rd row (REMOTE 2) code switches, and digital IC power supply and GND +5V2, GND2: 2nd row (REMOTE 1) and 4th row (REMOTE 2) code switches 2.9 Ambient Temperature 5 to 35°C (41 to 95°F), 85% or less and Humidity: 160 W × 35 H × 110 D mm 2.10 Dimensions: $(6.30 \text{ W} \times 1.38 \text{ H} \times 4.33 \text{ D in.})$ (Maximum Dimensions): 167 W × 60 H × 113 D mm $(6.57 \text{ W} \times 2.36 \text{ H} \times 4.45 \text{ D in.})$ (excluding the connection cable) 2.11 Weight: Approx. 0.7 kg (1.5 lbs) [Approx. 0.8 kg (1.8 lbs)] 2.12 Accessories: Instruction manual 1 сору Blanking caps 5 [4]

+5V2, GND2:

\$3228

GENERAL PRECAUTIONS

3.1 Unpacking

Upon receipt of the instrument, immediately unpack and inspect it for any damage which might have been sustained when in transportation. If any damage is found, immediately notify the transportation company and your Kikusui agent.

3.2 Power Source

For this instrument, two channels of power supplies (+5V1 - GND1, and +5V2 - GND2) should be supplied from the controlled equipment.

3.3 Environmental Conditions

Do not expose the instrument to direct sunlight. Do not place it near a heat generating equipment or other source of heat. Avoid operating the instrument in adverse environments (atmosphere with dust, gas or chemicals, or mechanical vibration) lest the longevity of the instrument should be shortened.

3.4 Others

The performance and other specifications of the instrument are subject to change without notice.

4. OPERATION METHOD

4.1 Explanation of Panel Items

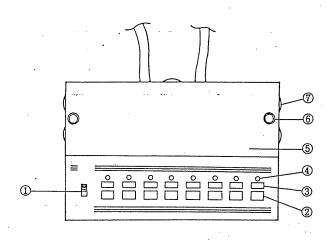


Figure 4-1. Front and Top Panel Items




Figure 4-2. Rear Panel Items

PANEL/REMOTE selector switch:

This switch selects between the PANEL mode for local control of the controlled equipment itself and the REMOTE mode for remote control. When the switch is set to the PANEL mode, the LED lamps 4 go off. When the switch is set to the REMOTE mode, the corresponding one of selected step indicator lamps 4 lights.

- (2) Step selector switches
- (3) Step numbers
- Selected step indicator lamps

Switches (2) are 8-key linked switches to select one of 8 steps. For the 8 keys, corresponding step numbers (3) and selected step indicator lamps (4) are provided. The corresponding lamp lights when switch (1) is set to the REMOTE mode. All lamps go off when all of switches (2) are set to off.

- 5 Top panel:
- (6) Top panel fixing-bottons:

The top panel can be removed by pulling the two top panel fixing-buttons, to perform programming or to change running directions of the remote control cable. A programming chart is posted on the back surface of top panel (5).

(7) Blanking caps:

These caps are used to close the unused cable holes. Be sure to close the unused holes to prevent ingression of dust and foreign matter.

(8) Remote control cable clamping-screws:

These screws are used to clamp the remote control cable. The remote control cable can be run in any one of the three directions.

Remote control cable:

The remote control cable is used to send the control signals between this instrument and the controlled equipment. It is approximately 2 m (6 ft) long.

(10) Remote control cable plug:

At the end of the remote control cable, the plug 10 (Amphenol 57-Series 57-50240 plug) is provided. For remote control, this plug should be connected to the receptacle (Amphenol 57-Series 57-40240 receptacle).

The RCO1-AVM has one set of remote control cable and plug; the RCO2-AVM has two sets of cables and plugs so that programming can be made for two sets of controlled equipment. The remote plugs are identified with markings of "REMOTE 1" and "REMOTE 2." The layout of the pins of the plug are as shown in Table 4-1.




Table 4-1. Layout of Pins of Remote Control
Cable Plug

4.2 Operation Method

Connect the remote control cable plug (10) to the receptacle of the equipment controlled.

Set the PANEL/REMOTE selector switch ① to the REMOTE state. As you turn on the power of the controlled equipment, the REMOTE LED lamp of the controlled equipment lights. At the same time, the LED lamp corresponding to the step number selected by the step selector switches ② lights and the data of the program corresponding to the selected step is delivered.

4.3 Programming Procedure

For programming of steps, proceed as explained in this section.

4.3.1 Explanation of Programming Chart

Remove the top panel (5) by removing the two top panel fixing-screws (6). A programming chart as shown in Table 4-2 is posted on the back surface of the top panel. The programming procedure is explained referring to the programming chart.

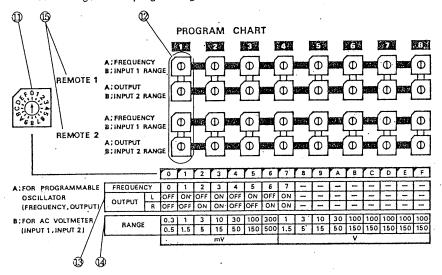


Table 4-2. Programming Chart

When the top panel is removed, 16-position rotary-type code switches (1) are accessible. The RCOl-AVM has total 16 of such switches laid out in the two top rows as shown in Table 4-2; the RCO2-ORC has total 32 of such switches laid out in the four rows.

Table (3) shows the items which are used to control Kikusui's Model ORC21 Programmable Controller, such as frequency addresses (0-7,8 types), combinations of ON/OFF states of R/L oscillator outputs (0-7,4 types), and positions corresponding to switch (1).

Table $\widehat{14}$ shows the items which are used to control Kikusui's Model AVM23R, AVM25R or other AC Voltmeter. The items are such as ranges (0 - F, 12 types) and positions of switch $\widehat{11}$.

Switches (12) correspond to step numbers (3).

Set the REMOTE 1 and REMOTE 2 switches (15) as explained in the following:

(1) RCO1-AVM

To control a Programmable Controller or an AC Voltmeter, connect the remote control cable plug to the receptacle of the equipment to be controlled.

- A: When controlling a Programmable Controller, the switches of the 1st row are for frequency addresses and those of the 2nd row are for combinations of ON/OFF of R/L oscillator outputs.
- B: When controlling an AC Voltmeter, the switches of the 1st' row are for INPUT 1 range setting and those of the 2nd row are for INPUT 2 range setting.

Two channels of power supplies and GND lines are provided. (See Section 2.9.)

(2) RC02-AVM

The remote control cable plugs are identified with markings "REMOTE 1" and "REMOTE 2". They can be connected to Programmable Controllers or AC Voltmeters. The switches of the 1st and 2nd rows are for the controlled equipment connected to REMOTE 1; those of the 2nd and 4th rows are for that connected to REMOTE 2.

- A: When controlling a Programmable Controller, the switches of the 1st or 3rd rows are for frequency addresses and those of the 2nd and 4th rows are for combinations of ON/OFF of—R/L oscillator outputs.
- B: When controlling an AC voltmeter, the switches of the 1st and 3rd rows are for the INPUT 1 range setting and those of the 2nd and 4th rows are for the INPUT 2 range setting.

Two channels of power supplies and GND lines are provided. (See Section 2.9.)

4.3.2 Example of Programming

An example of programming is introduced here for a case that Model RCO2-AVM Remote Controller is used to control Kikusui's Model ORC21 Programmable Controller and Model AVM23R AC Voltmeter at the same time.

Connect the REMOTE 1 of the remote control cable plug (10) to the Programmable Controller and the REMOTE 2 to the AC Voltmeter., (The REMOTE 1 plug may be connected to the AC Voltmeter and the REMOTE 2 plug to the Programmable Oscillator. The above connections are only for the sake of explanation.)

Assume that, for step $\boxed{5}$ of the Remote Controller, the Programmable Oscillator is to be programmed for the frequency and level set for [2] A from the frequency addresses, and both [R] and [L] outputs are to be set on [ON] B. Also assume that the AC Voltmeter is to be programmed at the [0.3 mV] C range for the $[INPUT\ 1]$ and at the $[1\ V]$ D range for the $[INPUT\ 2]$.

Set the code switches as shown in Table 4-3. Turn on the powers of the Programmable Oscillator and AC Voltmeter. Set the PANEL/REMOTE selector switch (1) to the REMOTE state. Press 5 of step selector switch (2) so that the instrument is set to the programmed mode.

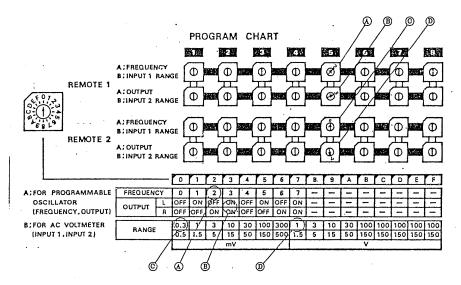


Table 4-3. Example of Programming

4.4 Notes for Noise and Longevity

- (1) Noise may be picked up when a remote-control setup is made. In such a case, move apart the Remote Controller, remote control cable and controlled equipment from equipment which probably is the source of noise, and provide separate power supplies.
- (2) The life expectancies of the switches of the Remote Controller are as follows:

(1) REMOTE/PANEL selector switches: 104 repetitions

② Step selector switches: 3×10^4 repetitions

or over

 \bigcirc Rotary-type code switches 2×10^4 steps or over for programming: