



King Saud University
Arabian Journal of Chemistry

www.ksu.edu.sa
www.sciencedirect.com



ORIGINAL ARTICLE

Detection of hippuric acid: A glue solvent metabolite, using a mobile test kit

Mohamad Raizul Zinalibdin *, Abdul Rahim Yacob ¹

Department of Chemistry, Faculty of Science, University Teknologi Malaysia, 81310 Skudai, Johor, Malaysia

Received 6 April 2010; accepted 9 September 2010

Available online 6 October 2010

KEYWORDS

Forensic Science;
Color test;
Glue;
G.S. Kit;
Hippuric acid;
Toluene;
Urine

Abstract Many testing kits for screening common drugs are widely used in Malaysia, such as the dip strip urine drug testing kit which is specified for detecting drug in abuser. However, currently there is no specific testing kit for screening urine samples to detect glue abusers. This research is dedicated to develop a specific color test method to emphasize the screening for glue abusers, known as G.S. Kit. It contains benzenesulphonyl chloride, pyridine and distilled water. The urine sample is mixed with pyridine and benzenesulphonyl chloride and followed by distilled water. A positive result will be in the form of a color reaction from yellow to red. This novel G.S. Kit would be quite useful for the screening and detection of glue sniffing and toluene abusing qualitatively, as a way of helping National Anti Drug Agency, Department of Education and Royal Police of Malaysia in preventing glue sniffing from becoming a social pandemic.

© 2010 King Saud University. Production and hosting by Elsevier B.V. All rights reserved.

1. Introduction

Toluene is also known as methyl benzene or phenyl methane. It is a clear and water insoluble liquid with a distinguished

sweet smell of the existing benzene compound (Ikeda et al., 1990). This chemical is widely used as an organic solvent in printing, painting, automotive, shoemaking, adhesive material and pharmaceutical industries (Serap et al., 2001). Normally, toluene is found in many products including paint and contact adhesives as a solvent. Besides that, some grades of toluene contain traces of xylene and benzene (Ikeda et al., 1990). It is also a common substance in glue and paint thinner that are sniffed by drug abusers.

Toluene abuse via glue sniffing is a growing problem and is considered nowadays as drug abusing in Malaysia. Even though it is an alternative to drugs, the national registry of abusers in Malaysia does not require the reporting of glue sniffers thus, there is no national statistics on the extent and nature of the problem (Sharifah, 1990). Based on newspaper articles, three teenagers aged 18–20 were found dead near a school in Cheras, Kuala Lumpur and Police found three cans of glue nearby (Jasmine, 2005). By the information from the newspapers and electronic media it is feared that glue sniffing problem

* Corresponding author. Tel.: +60 6012 7357660; fax: +60 607 2238366.

E-mail addresses: tikar_ajaib@yahoo.co.uk (M.R. Zinalibdin), manrahim@kimia.fs.utm.my (A.R. Yacob).

¹ Tel.: +60 607 5534505; fax: +60 607 5566162.



added to 0.25 mL pyridine and 0.1 mL BSC with 1.0 mL distilled water.

2.4. Determination of hippuric acid in urine using G.S. Kit

2.3.4. Sample selection

The samples were received from screening urine samples from students in secondary schools around Johor Bahru, Malaysia.

2.3.5. Manual instructions of G.S. Kit

- 0.1 mL urine samples and 2.0 mg/mL of hippuric acid standard were pipetted into the sample bottles.
- 0.25 mL pyridine 98% was added to the sample bottles containing urine and hippuric acid standard.
- 0.1 mL benzenesulphonyl chloride 98% and 1 mL of distilled water were added to the mixtures.
- Lastly, the mixture color of the mixture changes from yellow to red if hippuric acid is present in the urine samples. The color of the original urine samples was compared to the hippuric acid standard to detect glue abuse.

2.3.6. Safety precautions

- The G.S. Kit is to be stored at room temperature.
- The person conducting the analysis should wear a safety mask along with safety glove as a safety precaution from chemical exposure.
- The analysis must be conducted at the lab or open space with a good ventilation system.
- The mobile kit must be stored at an appropriate place away from the children.

3. Results and discussion

3.1. G.S. Kit-mobile test kit

3.1.1. G.S. Kit

The G.S. Kit-mobile test kit contains chemicals such as benzenesulphonyl chloride, pyridine and distilled water in 10 mL amber bottles, 20 sets of 5 mL sample bottles, a micro pipette, a pasteur pipette, rubber teat and pipette tips along with the standard series color chart of hippuric acid concentrations. Other than that, a manual instruction and safety precaution

booklet on how to use the kit, mask and rubber glove were also provided. Fig. 1 illustrates a picture of the G.S. Kit.

3.1.2. Standard series color chart of hippuric acid concentration

A light yellow color appears if the sample contains a low concentration of hippuric acid. The yellow color turns red as the concentration of hippuric acid increases. If there is no hippuric acid in the sample, the mixture will become colorless and transparent. The color change between 0.125 and 3.0 mg/mL hippuric acid standards is shown in Fig. 2. The result of the urine samples was compared to the series of the color chart. Limit of detection (LOD) hippuric acid using color test method is 0.125 mg/mL. There is no color change in the mixture even though the analysis is repeated several times.

3.2. Result of screening urine samples

3.2.1. Screening urine sample using color test method

The color test for screening urine sample is shown in Fig. 3 by using the G.S. Kit. If there is no presence of hippuric acid in urine sample, the mixture becomes colorless and transparent. The urine samples A and B illustrated light red color similar to the color of the standard hippuric acid of 2.0 mg/mL. Thus proving that hippuric acid is present in these samples. The figure shows the color change without adding distilled water and is useful only to differentiate the positive and negative results but not the concentration of hippuric acid present. Because of this, Yoshida et al. (2001) added distilled water to differentiate the red color development if high concentrations of hippuric acid are present and it is shown clearly in Fig. 5.

The reaction of the color test method gives the red color development. Fig. 4 shows the chemical equation between benzenesulphonylchloride, pyridine and hippuric acid. In the equation, the chloride of benzenesulphonylchloride attacks the amine group or hydroxyl group of hippuric acid and forms an ester or ether group. Then, the chloride atom forms hydrochloric acid. Pyridine is an acid indicator for this reaction as well as phenolphthalein which develops the red color. that indicates the presence of hippuric acid in the urine samples.

Although the red color formed was from reaction of pyridine with hydrochloric acid it cannot distinguish the level of hippuric acid concentration. Thus, Yoshida et al. (2001) came up with a new solution of adding distilled water to the mixture. Distilled water is slightly acidic and it has hydrogen ion (H^+), hydroxide ion (OH^-) and some metals. By addition of distilled

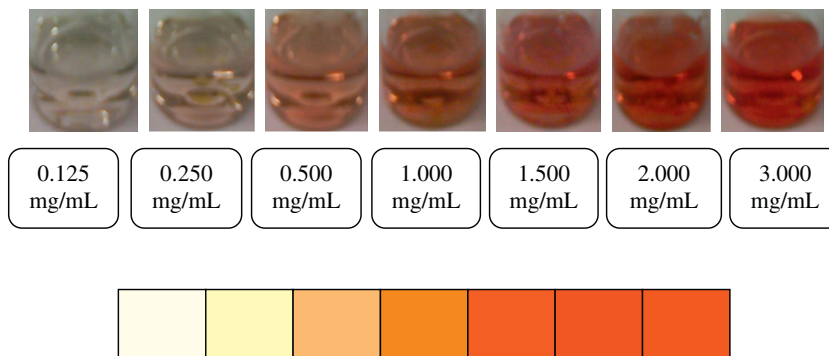


Figure 2 Standard series color chart of hippuric acid concentrations.

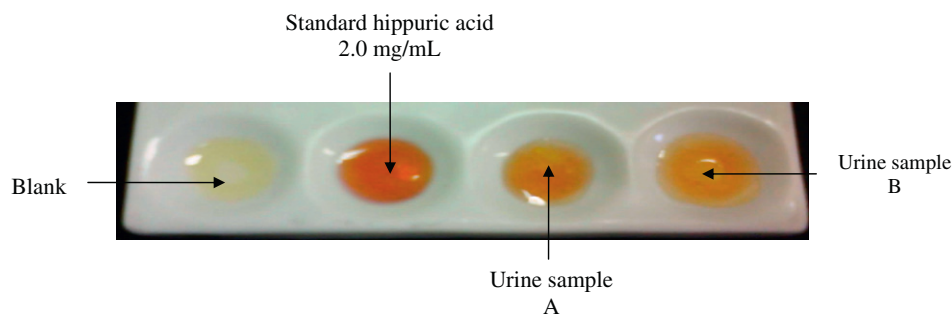


Figure 3 Color test for screening urine sample.

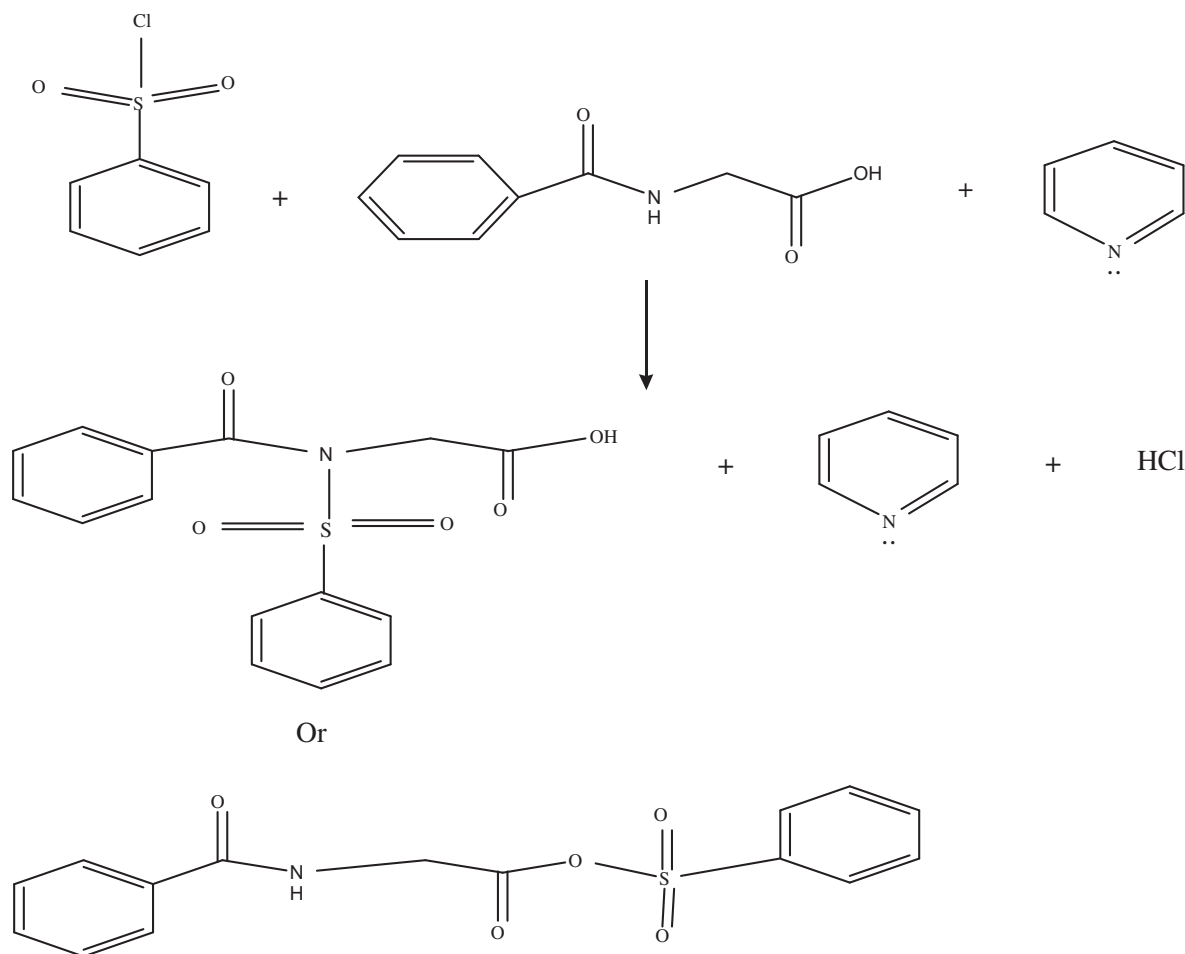


Figure 4 Chemical equation of color test method.

water, acidic value of the mixture will increase and the red color formed is based on the hippuric acid concentration.

3.3. Result of screening sample at secondary school

Forty four students were involved in the screening urine test using G.S. Kit at a secondary school in Johor Bahru. Four students gave positive results for hippuric acid in the urine samples while others gave negative results. At the same time, the National Anti Drug Agency was conducting a screening test for 5 drugs using the dip strip kit on the same samples and none of the students tested positive. The positive hippuric acid

sample was analyzed quantitatively using Ultra Violet Visible (UV-Vis) spectrometer. The color test reaction is shown in Fig. 5. Even though, the color reaction is quite useful for qualitative analysis, the color of the reaction mixture will fade gradually. So, semi quantification should be performed as soon as possible. The G.S. Kit is a fast tool for detecting glue abuse with the results obtained within 5 min.

3.3.1. Color test for hippuric acid using UV-Vis

The UV-Vis spectra of the mixtures were recorded at 300–700 nm using Perkin Elmer Ultra Violet Visible (UV-Vis). A color chart for the semiquantitation of hippuric acid was pre-

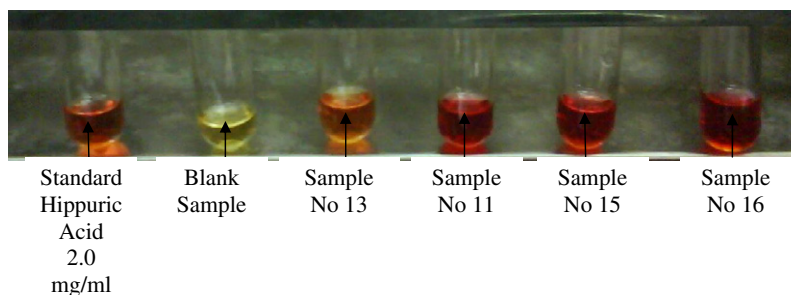


Figure 5 Color test for screening urine sample at the secondary school.

Table 1 Concentration of hippuric acid standard using color test method at 417 nm wavelength.

Concentration of hippuric acid	Absorbance
0.000	0.000
0.125	0.149
0.250	0.284
0.500	0.337
1.000	0.654
1.500	0.797
2.000	0.993
3.000	1.500
6.000	2.667

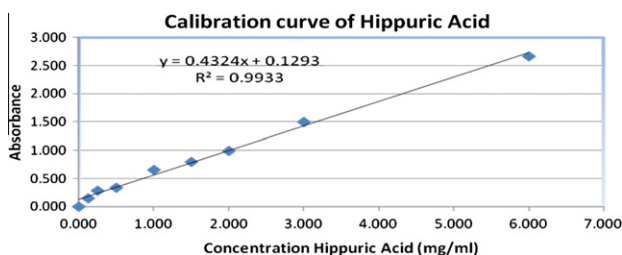


Figure 6 Calibration curve of hippuric acid using color test method.

pared using standard samples of 0.125, 0.25, 0.50, 1.0, 1.50, 2.0, 3.0 and 6.0 mg/mL hippuric acid. Table 1 shows the concentration of hippuric acid using color test method at wavelength 417 nm. From the table, it is obvious that the color test method has successfully determined the presence of hippuric acid at different concentrations relative to the intensity of red color developed by the mixture.

Fig. 6 demonstrates the calibration curve of hippuric acid using color test method with correlation value of hippuric acid concentration and absorbance. It is useful to determine hippuric acid concentration qualitatively.

Based on the screening urine test using G.S. Kit the result shows that four students gave the positive presence of hippuric acid that can be determined by calculation based on calibration curve equation. Calculated amount of hippuric acid in urine is shown in Table 2.

A few articles have defined the detected amount of hippuric acid to be considered as glue abuse. Yoshida et al. (2001) suggested that 2.0 mg/mL hippuric acid indicated high probability of being a glue sniffer while 1.0–1.5 mg/mL suggested the pos-

Table 2 Result of amount of hippuric acid using color test method by UV-Vis for screening urine sample at secondary school.

Sample number	Sample amount, mg/mL $\pm$ RSD*
	Hippuric acid
11	3.35 $\pm$ 0.03
13	1.40 $\pm$ 0.009
15	2.54 $\pm$ 0.01
16	3.00 $\pm$ 0.03

* Based on triplicate samples.

sibility of being a glue sniffer. Normal level of hippuric acid produced by the human body is 0.1 mg/mL per day.

Based on the stated definition, the results in Table 2 show the test for the positively tested students. Three of the students have high probability of being glue sniffers while one has the possibility of being a glue sniffer. From the qualitative and quantitative analysis of hippuric acid, it can be concluded that these 3 students may be positive glue sniffers and from this, it was proved that the G.S. Kit provides significant and accurate result, good linearity and detection limit comparable to UV-Vis instrument.

4. Conclusion

The color test method produced by the G.S. -mobile test kit is very useful, and fast with good linearity and accuracy. This kit is useful for detecting and screening glue sniffer's urine. Other than that, this kit has been patented by KASS SDN BHD as a patent product and the ID number is PI 20101467. The G.S. Kit might be used by National Anti Drug Agency and Royal Police of Malaysia for preventing glue abuse among students and teenagers.

Acknowledgments

Special thanks to National Anti Drugs Agency (AADK) for the collaboration in this research, and for financial support from Ministry of Science Technology and Innovation (MOSTI) and Department of Chemistry, Johor branch for full support.

References

- Ameno, K., Fuke, C., Ameno, S., Kirui, T., Sogo, K., Ijiri, I., 1989. A fatal case of oral ingestion of toluene. J. Sci. Int. 41, 255–260.

- Anderson, C.E., Loomis, G.A., 2003. Recognition and prevention of inhalant abuse. *Am. Fam. Phys.* 68, 869–874.
- Ikeda, N., Takahashi, H., Umetsu, K., Suzuki, T., 1990. The course of respiration and circulation in toluene sniffing. *J. Sci. Int.* 44, 151–158.
- Jasmine, S. Powerless to act on glue sniffing. *New Straits Times newspaper*. 2005 June 6th
- Serap, A.A., Pembe, O., Yusuf, K., Huseyin, K., Suheyla, E., 2001. Medicolegal aspects of blood–urine toluene and urinary ortho-cresol concentration in toluene exposure. *Turk. J. Med. Sci* 31, 415–419.
- Sharifah, M.T.F. Report of the Inhalant Abuse problem in Sarawak, East Malaysia. Paper presented at the Twelfth INFGO Conference Singapore, 1990 November 12–16.
- Umberger, C.J., Fiorese, F.F., 1960. Colorimetric method of hippuric acid. *J. Clin. Chem.* 72, 91–96.
- Yacob, A.R., Zinalibdin, M.R., 2009. Characterization using instrumentation of local glue related glue sniffing activity. *Ind. J. Med. Toxicol.* 3 (2), 58–64.
- Yacob, A.R., Zinalibdin, M.R., 2010. Spectrophotometry semiquantitation method hippuric acid in urine for demonstration of glue abuser. *Ind. J. Med. Toxicol.* 4 (1), 22–32.
- Yamazaki, K., Tanaka, E., Misawa, S., 1992. Urinary ortho-cresol concentrations as an indicator of toluene inhalation in glue sniffer. *J. Sci. Int.* 32, 215–223.
- Yoshida, M., Akane, A., Mitani, T., Watabiki, T., 2001. Simple colorimetric semiquantitation method of hippuric acid in urine for demonstration of toluene abuse. *J. Sci. Leg. Med.* 7, 198–200.
- Zuppi, C., Rosetti, D.V., Vitali, A., Vicenzoni, F., Giardin, B., Castagnola, M., Messina, I., 2003. Determination of urinary hippuric acid by micellar chromatography. *J. Chromatogr. B* 793, 223–228.