© 2009 Adis Data Information BV. All rights reserved.

Patient-Controlled Analgesia-Related Medication Errors in the Postoperative Period

Causes and Prevention

Jeff R. Schein, ¹ Rodney W. Hicks, ² Winnie W. Nelson, ³ Vanja Sikirica ⁴ and D. John Doyle ⁵

- 1 Ortho-McNeil Janssen Scientific Affairs, LLC, Raritan, New Jersey, USA
- 2 US Pharmacopeia, Rockville, Maryland, USA
- 3 Johnson & Johnson Pharmaceutical Services, Raritan, New Jersey, USA
- 4 Ethicon, Inc., Somerville, New Jersey, USA
- 5 Cleveland Clinic, Cleveland, Ohio, USA

Contents

Abstract	549
1. Analgesia as a Contributor to Patient Risk	551
2. Classification of Patient-Controlled Analgesia (PCA) Errors	551
2.1 Potential Causes of Human-Related PCA Errors	551
2.2 Potential Causes of Equipment-Related PCA Errors	553
3. Device and Medication Error Reporting Databases	554
3.1 Manufacturer and User Facility Device Experience (MAUDE) Database	554
3.2 MEDMARX® Database	554
4. Reducing PCA Medication Errors	555
5. Conclusions	556

Abstract

Patient-controlled analgesia (PCA) is a common and effective means of managing postoperative pain. Unfortunately, the complex processes and equipment associated with the setup, programming and administration of intravenous or epidural PCA have allowed it to become a significant source of preventable medication errors. These errors can be classified into two major categories: human (operator) errors and equipment errors (malfunctions). Such errors are potentially harmful to patients, time-consuming for hospital staff and costly for healthcare providers. The objective of this article is to describe PCA medication errors and examine systems and modalities that may help reduce the incidence of system-related errors. Data from the US FDA's Manufacturer and User Facility Device Experience (MAUDE) database indicate that 6.5% of intravenous PCA-related events were due to operator error. Most (81%) of these errors were due to pump misprogramming, of which almost half were associated with patient harm; 76.4% of adverse events were attributed to device malfunction (e.g. due to frayed wires or a crack in the drug cartridge), although only 0.5% of these were associated

with harm to patients. In a report based on data from MEDMARX®, a voluntary database that captures reports on medication errors, 7.9% of the PCA-related errors captured over a 5-year period were described as causing harm to patients. Technological advances, such as improved PCA pump designs based on ergonomic and cognitive engineering principles, the use of barcode technology and other 'smart pump' safety features, and new post-operative pain management modalities, may play a significant role in reducing the future incidence and severity of PCA medication errors.

An estimated 44 000-100 000 fatalities and 1.3 million injuries occur each year as a result of medical treatment.[1-3] Studies have shown that 19.4% of adverse events are treatment related. [1,3] Some of these are the result of medication errors, which are preventable mistakes that may occur at any point during the medication delivery process, including ordering, transcribing, dispensing and administering medication and patient monitoring.^[4] It has been reported that errors occur in 5.3% of all medication orders.^[2] Actual medication error rates, however, are likely to be higher, as most medication errors are not documented.^[5] Each year, medication errors result in approximately 7000 deaths, [2] as well as other serious adverse drug events (ADEs).

Although not all ADEs are the result of medication errors (e.g. predictable adverse effects accompanying drug treatment such as hair loss following chemotherapy), 30-50% of ADEs are attributable to this cause. [6,7] Additional consequences of medication errors in the hospital setting include prolonged patient hospitalization, consumption of staff time and increased resource utilization. For example, the annual incremental healthcare costs associated with medication errors in the US were estimated in 2006 to be approximately \$US3.5 billion.[8] Given this, and the fact that 1.33% of medication errors cause harm to the patient, [9] reducing the incidence of medication errors would significantly improve the current status of healthcare in the US.[10,11] Achieving significant reductions in medication error incidence rates is an important initiative that will require involvement from multiple sectors of the healthcare system.

Identifying the sources of medication errors is important to correct the causes. In the hospital

setting, patient-controlled analgesia (PCA) is a known source of errors, [9,12] especially in postoperative care. Primarily administered via intravenous (IV) or epidural administration routes, PCA is commonly and effectively used to manage acute pain.[13-20] This analgesic modality has revolutionized postoperative pain management by allowing patients control over their own pain relief, thereby reducing lapses in pain relief (analgesic gaps).[13,16,21,22] A meta-analysis[23] of 55 randomized controlled trials that evaluated PCA versus conventional analgesia found that PCA provided better pain control and increased patient satisfaction. In addition, PCA may be a more time-efficient option for nurses, allowing them time to take care of other patients rather than attending to analgesic delivery needs. However, while effective, PCA use has introduced new sources of medication errors. One analysis^[24] estimated that more than 13 million patients receive IV PCA in the US annually, and approximately 4.5% of those patients experience an error. One possible explanation for these errors is that IV and epidural PCA administration involve processes that require the coordination of several hospital departments, and the programming of PCA pumps requires attention to detail.^[25] Furthermore, PCA pumps utilize different types and dosages of opioids, which are described by the Institute for Safe Medication Practices as 'high-alert' medications and are associated with a significant number of medication errors.[26] Combining the 'high alert' status of opioids with the complex equipment and processes associated with epidural and IV PCA presents an opportunity for numerous medication errors, some potentially fatal, resulting from human- or equipment-related factors. The objective of this

review article is to describe PCA medication errors and examine systems and modalities that may help reduce the future incidence of these errors.

1. Analgesia as a Contributor to Patient Risk

Many types of medication errors occur with analgesia treatment. One review of the biomedical literature published in 2003 indicated that analgesics were associated with 12.8% of all preventable ADEs;^[27] only cardiovascular drugs (17.9%) and psychoactive and CNS agents (15.3%) were associated with more preventable ADEs. Opioids are the most common analgesics used during PCA treatment and are associated with more analgesic-related medication errors than any other drug class.[27-35] In particular, opioids have been cited as the most common 'intended' analgesics in instances when an incorrect drug was administered to patients.^[36] In 2006, the 5 Million Lives Campaign, an initiative intended to reduce medication-related harm for 5 million patients between December 2006 and December 2008, noted opioids as one of four groups of medications (along with anticoagulants, insulin and sedatives) that are particularly likely to cause harm to patients, even when used as intended. [37] Common ADEs associated with opioids that may occur with correct or erroneous administration include nausea and vomiting, pruritus and constipation.[38,39] However, opioids may also be associated with respiratory depression, which can be fatal.^[23] The incidence of respiratory depression in patients treated with opioids via PCA ranges from 0.1% to 3.9%, depending on the opioid used and the method of administration.[17]

While opioids may be associated with ADEs and pose an inherently increased risk of medication errors, opioid use during PCA treatment in particular may be associated with a number of unique medication errors.^[14,17,40-51] As illustrated in figure 1, the administration of PCA requires a prescription from a licensed prescriber, preparation by the pharmacist, the assembly and programming of a PCA pump by a nurse or physician, and PCA pump activation by the

patient.^[25] As a result, there are multiple steps during drug delivery at which various types of medication errors (e.g. administration of the wrong analgesic, PCA pump misprogramming or false triggering of the PCA pump) may occur.

2. Classification of Patient-Controlled Analgesia (PCA) Errors

Having identified PCA as a frequent source of medication errors, it is then important to classify the various types of errors that may occur. By doing so, one can pinpoint areas of system-. process- or device-related medication errors that can be targeted to reduce future errors. The National Coordinating Council for Medication Error Reporting and Prevention Taxonomy of Medication Errors describes five main causes of medication errors: communication, name confusion, labelling, human factors and packaging /design.^[52] While appropriate for categorizing the causes of medication errors on a general level, this taxonomy is less suited for categorizing PCArelated errors, a significant source of which is the technology used to deliver PCA. Accordingly, Doyle^[53] previously described a taxonomy for categorizing potential PCA-related safety hazards using 13 different error groups (table I). By definition, not all of these PCA-related hazards have the potential to result in true medication errors (for example, unknown patient sensitivity to opioids or pump reprogramming with criminal intent). However, failure to recognize or avoid most of these hazards can result in medication errors and potential harm to the patient. Ultimately, the hazards encountered with PCA use can be divided into two main overarching categories: human errors and equipment errors.

2.1 Potential Causes of Human-Related PCA Errors

Errors in prescribing or ordering contribute substantially to preventable ADEs.^[28] In a prospective observational study of patients in a medical/surgical intensive care unit,^[54] most preventable ADEs occurred during drug

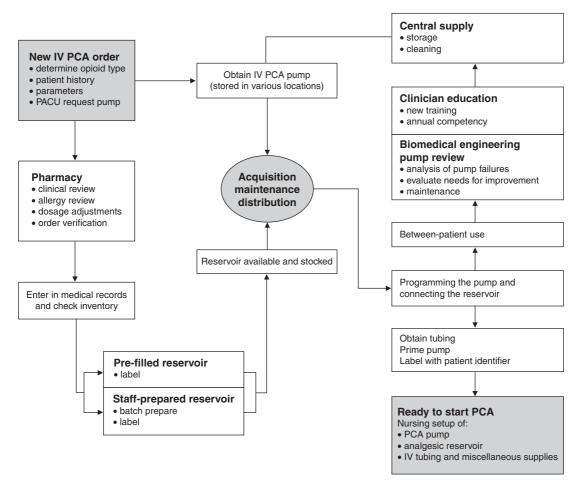


Fig. 1. Steps involved in the administration of intravenous (IV) patient-controlled analgesia (PCA). [25] This diagram demonstrates the complexity of the process of administering IV PCA, from the starting point of patient screening to the endpoint of actual administration (reproduced from Hutchison et al., [25] with permission from Hospital Pharmacy). **PACU** = postanaesthesia care unit.

prescription (77%). A larger prospective study of 4031 adult patients admitted to 11 medical and surgical units in two tertiary-care hospitals over a 6-month period likewise found that a majority (56%) of medication errors occurred at the ordering stage, with incorrect dosing as the most common ordering error, followed by inappropriate medication choice, prescription of a medication to which the patient was allergic, ordering at the wrong frequency of administration, and failure to anticipate a drug-drug interaction. [28] Execution of treatment is another step in the process of providing medication where

human error may occur. In fact, in a prospective observational study of critically ill patients, ^[55] the most common of 277 serious medical errors were associated with both the medication ordering process and execution of treatment, including wrong dosage (22.4%) and duplicate medication orders (7.6%).

Once a medication is ordered, errors in the hospital pharmacy's medication ordering and dispensing process may contribute to medication errors. Such errors include a failure to identify provider ordering errors (e.g. incorrect dosing or prescription of a medication to which a patient is

allergic). While the biomedical literature does not specifically identify pharmacy ordering and dispensing as a source of PCA-related errors, mistakes in ordering and dispensing are a notable source of medication errors in general^[28,56,57] and are errors to which current IV and epidural PCA modalities are not immune. Most hospital prescriptions are filled in a two-step process, in which pharmacy technicians fill drug orders and pharmacists verify the orders.^[56] This protocol is effective for catching many prescription errors before the product leaves the pharmacy. Reported rates of pharmacy dispensing errors range from 0.0041% to 3.6%.^[28,56,58-60]

However, errors may still occur despite this two-step process and can have significant and even fatal consequences. In one observational study of a tertiary-care hospital pharmacy, 3.6% of all orders were filled improperly by pharmacy technicians, and 0.75% of all orders were approved to leave the pharmacy with undetected errors. [56] The errors identified in that study included dispensing of incorrect medications (36%), incorrect medication strength (35%) and incorrect dosage form (21%). [56] Given the annual number of medication orders filled by the hospi-

Table I. Patient-controlled analgesia (PCA)-related safety hazards^[53]

Use of wrong analgesic or wrong analgesic cartridge

Accidental pump misprogramming

False triggering (e.g. PCA button short circuit)

False triggering by proxy (e.g. activation of PCA pump by nurse/visitors)

Drug accumulation in IV deadspace

Runaway fluid column due to 'siphoning' or other means

PCA pump malfunction due to hardware failure

PCA pump malfunction due to software design error^a

Retrograde flow of PCA analgesic into a second IV set due to catheter blockade

Bad medical judgement in formulating a PCA prescription or order Anaphylaxis

Unknown sensitivity of the patient to opioids resulting in respiratory depression

Reprogramming with criminal intent^a

Hazard is theoretical at this time.

IV = intravenous.

tal pharmacy where the study was conducted (6 million), these data suggested that 45 000 dispensing errors would have left the pharmacy each year, with 10 600 having the potential for patient harm.^[56]

Finally, human-related PCA medication errors may result from errors that occur during pump programming or pump activation.[7,14,17,40-46,49,50] The use of PCA pumps is relatively complex^[25] and often requires significant training for proper setup and monitoring. Complicating the situation, poorly designed interfaces on some PCA pumps have been cited as a significant source of PCA pump-related human errors.[47,48,61-63] Because of the complexity of PCA pumps, stringent protocols are required to help reduce the risk of errors; dangerous errors, including the administration of an incorrect drug, may result when these protocols are not followed. [17] Other sources of human error include accidental activation of drug delivery by the patient or family members, [64,65] PCA pump activation by proxy (i.e. someone other than the patient),^[51] misunderstanding of device use by the patient^[66] and poor judgement by physicians in prescribing drugs or considering the risk of a known ADE,^[53] all of which have the potential to result in preventable opioid-related ADEs. Variability in drug names, concentrations, dose limits and administration practices^[67] also make it difficult to standardize PCA safety recommendations, and have the potential to result in the administration of the wrong drug, the wrong dose, the wrong infusion time and/or the wrong lockout interval.

2.2 Potential Causes of Equipment-Related PCA Errors

Pump malfunction or other equipment-related errors are another significant source of PCA medication errors.^[68-71] Potential causes of equipment-related PCA errors include short circuits caused by frayed wires,^[72] poorly designed pump user interfaces,^[73] drug accumulation in IV deadspace^[74] and siphoning due to a crack in the drug cartridge,^[75] any of which may lead to either false triggering or accidental drug delivery by the PCA device. Malfunctions of PCA pumps have

also been reported when they were used in a hyperbaric environment^[76] or in close proximity to an MRI machine.^[77] All of these errors have the potential to result in under- and/or over-dosing.

3. Device and Medication Error Reporting Databases

To determine the impact of the many theoretical hazards associated with PCA use, medication error databases may be utilized to determine the actual significance and incidence of PCA-related errors. There are two major error-reporting databases that can be used to track the incidence, type and severity of PCA-related medication errors: (i) the US FDA's Manufacturer and User Facility Device Experience (MAUDE) database; and (ii) the United States Pharmacopeia (USP) MEDMARX® database.

3.1 Manufacturer and User Facility Device Experience (MAUDE) Database

The FDA Medical Device Reporting regulations require device manufacturers and user facilities to report any postmarketing complaints or adverse events related to device malfunctions, including serious injuries and deaths.^[78] The MAUDE database is the publicly available repository of these reports.^[78] Each error report includes information about patient outcomes that result from the event, information about the device used during the event and narrative text provided by the device reporter and/or device manufacturer about the events, their causes, patient outcomes and results of any manufacturer device testing. In order to assess the nature of IV PCA-related error reports, an analysis of the MAUDE database between January 2002 and December 2003 was undertaken.^[79] Of the 2009 IV PCA-related events identified, 1590 events (79.1%) were possibly related to the PCA device. Specifically, 76.4% of events were suspected to have resulted from device defects, including a defective reed switch; a defective motor; and battery, display board or software problems.^[79] Pump manufacturers confirmed 64.9% of the suspected device malfunctions. Of the 2009 IV

PCA-related reports, 131 (6.5%) were suspected to be due to operator (i.e. human) error; an overwhelming number of these (106) were the result of PCA pump programming errors.^[79] Upon further review of the error reports to determine patient outcomes associated with IV PCA-related events, only 0.5% of events possibly related to device malfunction were associated with harm to the patient; conversely, 48.1% (63 of 131) of events related to operator error and 29.1% (48 of 165) of events related to over-delivery of drug by indeterminate cause were associated with harm to the patient. Collectively, these data suggest that equipment errors are the leading cause of PCA-related medication errors recorded in the MAUDE database. However, the MAUDE database may not have fully captured events that were considered to be unrelated to device malfunction, such as prescribing errors.

3.2 MEDMARX® Database

MEDMARX is a voluntary and anonymous online medication error reporting database that contains over 1.3 million reported medication errors.[80] One of the largest voluntary reporting databases in the US, MEDMARX was developed by the USP and unlike the MAUDE database, which only records device-related errors, receives reports about any type of medication error, including those that might be devicerelated. In one analysis,[81] the USP examined the frequency and type of PCA-related errors reported during a 5-year period (1998-2003) and found that a total of 5377 PCA-related errors were reported during this timeframe. Of these, 7.9% were described as having caused harm to the patient. This frequency is 3.5-fold greater than the average overall harm rate for MEDMARX errors.^[81] The most common PCA-related errors identified by the MEDMARX system included improper dose/quantity (38.9%), unauthorized drug (18.4%) and omission error (17.6%).^[81]

In a more recent analysis of the MEDMARX database,^[82] the frequency, type and cause of PCA-related errors reported from 2000 to 2005 were examined. Of 919 241 errors recorded in the database during this time period, 9571 involved

PCA. The most common causes of PCA-related errors included human factors (69.8%) and equipment-related factors (19.5%). Events that resulted in patient harm were more common for PCA-related errors (6.5% of events) compared with non-PCA-related errors (1.5% of events); therefore, the overall risk of harm was 4.3-fold higher for PCA-related errors compared with non-PCA-related errors. [82] Like the observations in the aforementioned MAUDE database analysis, [79] these findings suggest that improvements to current PCA processes and modalities are needed to reduce the incidence of medication errors.

4. Reducing PCA Medication Errors

The Institute of Medicine has suggested that the majority of medication errors ultimately result from failure of the healthcare system as a whole. [2] Improving patient safety requires system-wide changes. Innovations and improvements to existing PCA practices, the development of new PCA modalities and the evolution of computer pump technology will all be likely to play a role in reducing the incidence and severity of PCA-related medication errors in the future. New PCA modalities should aim to reduce system-related errors rather than only addressing the human-related errors that may occur.

Advances in infusion pump technology are important for reducing IV infusion pump-related medication errors. [83,84] For example, 'smart' infusion pumps have been developed to help reduce the risk of pump programming errors. These pumps provide feedback to the programmer regarding drug doses and infusion rates and have drug libraries incorporated into their programs. [83,84] Even so, the potential for medication errors is not completely eliminated with smart pump technology. This was demonstrated when one smart IV pump (ALARIS Medical Systems [now Cardinal Health] Guardrails, version 5.0, Dublin, OH, USA) was subjected to failure modes and effects analysis, a common human factors method used to prospectively isolate and remove known and potential flaws from a system, process or equipment design before it reaches the

user.^[85] For example, while the new smart IV pump design reduced sources of incorrect dosing, errors due to tubing misplacement were identified that could cause over- or under-infusion of the drug and were not evident in a non-smart IV pump (Deltec 3000, Deltec Inc. [now Smiths Medical MD, Inc.], St Paul, MN, USA).^[85] This case example illustrated the challenges associated with new complex pump technology, namely that intended improvements in design may bring about unintended new hazards.

The development of new postoperative pain management modalities that move away from infusion pumps may address the drawbacks of current techniques and potentially reduce medication errors. One example of such a modality is the needle-free, preprogrammed, self-contained fentanyl HCl iontophoretic transdermal system (fentanyl ITS; IONSYSTM, Ortho-McNeil, Inc., Raritan, NJ, USA). As described in section 2.1, the use of current PCA pump modalities is complex, requiring the coordination of multiple steps between several hospital departments for the administration of analgesia, such as pump acquisition, maintenance, distribution and setup; drug reservoir ordering and acquisition; and training of hospital staff on proper programming and maintenance of the system.^[25] In contrast, the design of fentanyl ITS eliminates the risk of programming errors and pharmacy mistakes, and substantially reduces the number of steps and hospital departments involved.

In order to compare the potential of new PCA modalities to reduce the risk of medication errors, it is useful to use models of human cognition, such as Rasmussen's 'skills-rules-knowledge' model, [86] the cognitive levels of which span the spectrum from automatic ('skills'-based) to analytical ('knowledge'-based). Using this model, two broad categories of behaviour requiring different levels of cognitive demand can be identified: 'analytical'- or knowledge-based behaviour and 'perceptual'- or skills- and rules-based behaviour. [86] Based on cognitive demands, the administration of IV PCA requires working at the 'knowledge-based' or 'analytical' level, which is generally slow, demanding, serial and more error-prone. However, using a modality such as

fentanyl ITS promotes working at the 'perceptual-based' level, which is generally fast, effortless and less error prone.^[86]

The use of computers and information technology has also been suggested to be one of the primary ways to reduce the incidence of medication errors. [1,87-93] Computerized physician order entry systems allow physicians to order medication electronically (as opposed to handwriting orders), help standardize clinical practice, improve interdepartmental communication, and capture data for tracking and research purposes.[90,91] Clinical decision support systems aid physicians in making decisions regarding drug choice and dosage regimens, and may incorporate patient- and pathogen-specific information as well.^[89] Computerized drug allergy checking systems show promise in being able to significantly reduce the incidence of preventable allergic reactions, [90,94,95] and barcode technology has been shown to substantially decrease dispensing errors and reduce the risk of potential ADEs. [92] Alerts issued by barcode technology have also been shown to limit administration errors by reducing errors associated with giving the incorrect medication, treating the wrong patient or giving medication at the wrong time. [92,96]

Technological advancements, such as smart pumps, fentanyl ITS and improved information technology, have the potential to significantly decrease the incidence of PCA-related medication errors. However, it is important to note that the complete elimination of errors may not be feasible. The key to reducing medication errors in the future is to minimize the opportunities for their occurrence by limiting the requirement of hospital staff members to work at the 'knowledge-based' or 'analytical' level, and by implementing systems and modalities that promote working at the 'perceptual-based' level, which, by nature, will better synchronize mechanical design with innate human cognition processes.

5. Conclusions

Medication errors associated with PCA administration are a significant source of preventable patient morbidity, mortality and hospital resource

utilization. Many PCA-related errors are particularly dangerous because the medications involved (i.e. opioids) have narrow therapeutic indexes, and relatively small mistakes in dosing concentrations or lockout intervals can have serious or even fatal consequences. In addition, patients are generally in a medically vulnerable state when undergoing PCA treatment, which may limit their ability to alert hospital staff members when something is wrong.

Many PCA-related medication errors result from human errors, highlighting the potential safety hazards of PCA modalities that have a complex design, as well as the need for system-wide improvement. Technological advances, such as improved PCA infusion pumps and new post-operative pain management modalities, may play a significant role in reducing the future incidence and severity of PCA medication errors. Increased use of computerized ordering systems and data-bases may also provide insight into the sources of PCA medication errors and may eventually lead to improved guidelines and standard practices for limiting their incidence.

Acknowledgements

Declaration of conflicts of interest: Jeff R. Schein is an employee of Ortho-McNeil Janssen Scientific Affairs, LLC. Rodney W. Hicks has worked for US Pharmacopeia. Winnie W. Nelson served as a consultant for Ortho-McNeil Janssen Scientific Affairs, LLC, during the development of this article and is currently an employee of Johnson & Johnson Pharmaceutical Services. Vanja Sikirica is an employee of Ethicon, Inc., a Johnson & Johnson company, and holds stock in Johnson & Johnson. John Doyle is an employee of the Cleveland Clinic, Cleveland, Ohio, USA, and has no affiliation with any pharmaceutical company or conflicts of interest to report.

Editorial assistance for the writing of this article was provided by Lara Primak, MD, of MedErgy and was supported by Ortho-McNeil Janssen Scientific Affairs, LLC.

References

- Kaushal R, Barker KN, Bates DW. How can information technology improve patient safety and reduce medication errors in children's health care? Arch Pediatr Adolesc Med 2001; 155 (9): 1002-7
- Kohn LT, Corrigan JM, Donaldson MS, et al. To err is human: building a safer health system. Washington, DC: National Academy Press, 1999

- Leape LL, Lawthers AG, Brennan TA, et al. Preventing medical injury. QRB Qual Rev Bull 1993; 19 (5): 144-9
- Gandhi TK, Seger DL, Bates DW. Identifying drug safety issues: from research to practice. Int J Qual Health Care 2000; 12 (1): 69-76
- Flynn EA, Barker KN, Pepper GA, et al. Comparison of methods for detecting medication errors in 36 hospitals and skilled-nursing facilities. Am J Health Syst Pharm 2002; 59 (5): 436-46
- Bates DW. Medication errors. How common are they and what can be done to prevent them? Drug Saf 1996; 15 (5): 303-10
- Morimoto T, Gandhi TK, Seger AC, et al. Adverse drug events and medication errors: detection and classification methods. Qual Saf Health Care 2004; 13 (4): 306-14
- Committee on Identifying and Preventing Medication Errors, Aspden P, Wolcott J, et al. Preventing medication errors: quality chasm series. Washington, DC: The National Academies Press, 2007
- Hicks RW, Becker SC, Cousins DD. MEDMARX® data report: a chartbook of medication error findings from the perioperative settings from 1998-2005. Rockville (MD): USP Center for the Advancement of Patient Safety, 2006
- Avorn J. Putting adverse drug events into perspective. JAMA 1997; 277 (4): 341-2
- Avorn J. Dangerous deception-hiding the evidence of adverse drug effects. N Engl J Med 2006; 355 (21): 2169-71
- Hicks RW, Becker SC, Windle PE, et al. Medication errors in the PACU. J Perianesth Nurs 2007; 22 (6): 413-9
- Etches RC. Patient-controlled analgesia. Surg Clin North Am 1999; 79 (2): 297-312
- Grass JA. Patient-controlled analgesia. Anesth Analg 2005;
 Suppl. 5: S44-61
- Lebovits AH, Zenetos P, O'Neill DK, et al. Satisfaction with epidural and intravenous patient-controlled analgesia. Pain Med 2001; 2 (4): 280-6
- Lehmann KA. Patient-controlled analgesia: an efficient therapeutic tool in the postoperative setting. Eur Surg Res 1999; 31 (2): 112-21
- Macintyre PE. Safety and efficacy of patient-controlled analgesia. Br J Anaesth 2001; 87 (1): 36-46
- Walder B, Schafer M, Henzi I, et al. Efficacy and safety of patient-controlled opioid analgesia for acute postoperative pain: a quantitative systematic review. Acta Anaesthesiol Scand 2001; 45 (7): 795-804
- Sidebotham D, Dijkhuizen MR, Schug SA. The safety and utilization of patient-controlled analgesia. J Pain Symptom Manage 1997; 14 (4): 202-9
- Bennett RL, Batenhorst RL, Bivins BA, et al. Patientcontrolled analgesia: a new concept of postoperative pain relief. Ann Surg 1982; 195 (6): 700-5
- Carr DB, Reines HD, Schaffer J, et al. The impact of technology on the analgesic gap and quality of acute pain management. Reg Anesth Pain Med 2005; 30 (3): 286-91
- Panchal SJ, Damaraju CV, Nelson WW, et al. Systemrelated events and analgesic gaps during postoperative pain management with the fentanyl iontophoretic transdermal system and morphine intravenous patient-controlled analgesia. Anesth Analg 2007; 105 (5): 1437-41

- Hudcova J, McNicol E, Quah C, et al. Patient controlled opioid analgesia versus conventional opioid analgesia for postoperative pain. Cochrane Database Syst Rev 2006; (4): CD003348
- Meissner B, Hicks RW, Sikirica V, et al. The rate and costs attributable to intravenous patient-controlled analgesia errors. Hosp Pharm 2007; 44 (4): 312-24
- Hutchison R, Anastassopoulos K, Vallow S, et al. Intravenous patient-controlled analgesia pump and reservoir logistics: results from a multicenter questionnaire. Hosp Pharm 2007; 42 (11): 1036-44
- 26. Vaida AJ, Urbanski B, Grissinger M, et al. PCA Drug Libraries: designing, implementing, and analyzing CQI reports to optimize patient safety [online]. Available from URL: http://www.ismp.org/profdevelopment/PCADrugLib rariesforwebce.pdf [Accessed 2008 May 15]
- Kanjanarat P, Winterstein AG, Johns TE, et al. Nature of preventable adverse drug events in hospitals: a literature review. Am J Health Syst Pharm 2003; 60 (17): 1750-9
- Bates DW, Cullen DJ, Laird N, et al. Incidence of adverse drug events and potential adverse drug events: implications for prevention. ADE Prevention Study Group. JAMA 1995; 274 (1): 29-34
- Bates DW, Boyle DL, Vander Vliet MB, et al. Relationship between medication errors and adverse drug events. J Gen Intern Med 1995; 10 (4): 199-205
- Cullen DJ, Sweitzer BJ, Bates DW, et al. Preventable adverse drug events in hospitalized patients: a comparative study of intensive care and general care units. Crit Care Med 1997; 25 (8): 1289-97
- Cullen DJ, Bates DW, Leape LL. Prevention of adverse drug events: a decade of progress in patient safety. J Clin Anesth 2000; 12 (8): 600-14
- Gray SL, Sager M, Lestico MR, et al. Adverse drug events in hospitalized elderly. J Gerontol A Biol Sci Med Sci 1998; 53 (1): M59-63
- Kaushal R, Bates DW, Landrigan C, et al. Medication errors and adverse drug events in pediatric inpatients. JAMA 2001; 285 (16): 2114-20
- Pearson TF, Pittman DG, Longley JM, et al. Factors associated with preventable adverse drug reactions. Am J Hosp Pharm 1994; 51 (18): 2268-72
- Thomas EJ, Studdert DM, Burstin HR, et al. Incidence and types of adverse events and negligent care in Utah and Colorado. Med Care 2000; 38 (3): 261-71
- Currie M, Mackay P, Morgan C, et al. The Australian Incident Monitoring Study. The 'wrong drug' problem in anaesthesia: an analysis of 2000 incident reports. Anaesth Intensive Care 1993; 21 (5): 596-601
- Institute for Healthcare Improvement. 5 Million Lives Campaign. Getting started kit: prevent harm from highalert medications. How-to guide. Cambridge (MA): Institute for Healthcare Improvement, 2006
- Chevlen E. Opioids: a review. Curr Pain Headache Rep 2003; 7 (1): 15-23
- Inturrisi CE. Clinical pharmacology of opioids for pain. Clin J Pain 2002; 18 (4 Suppl.): S3-13
- Abbott PCA Plus II patient-controlled analgesic pumps prone to misprogramming resulting in narcotic overinfusions [hazard report]. Health Devices 1997; 26 (9-10): 389-91

- Brown SL, Bogner MS, Parmentier CM, et al. Human error and patient-controlled analgesia pumps. J Intraven Nurs 1997; 20 (6): 311-6
- 42. Eade DM. Patient-controlled analgesia-eliminating errors. Nurs Manage 1997; 28 (6): 38-40
- ECRI. Medication safety: PCA pump programming errors continue to cause fatal overinfusions [hazard report]. Health Devices 2002; 31 (9): 342-6
- Grissinger M. Safety issues with patient-controlled analgesia, part 1: causes of errors. Pharm Today 2003; 21
- Grissinger M. Safety issues with patient-controlled analgesia, part 2: how to prevent errors. Pharm Today 2003; 16
- Vicente KJ, Kada-Bekhaled K, Hillel G, et al. Programming errors contribute to death from patient-controlled analgesia: case report and estimate of probability. Can J Anesth 2003; 50 (4): 328-32
- Doyle DJ, Vicente KJ. Patient-controlled analgesia. CMAJ 2001; 164 (5): 620-1
- Lin L, Isla R, Doniz K, et al. Applying human factors to the design of medical equipment: patient-controlled analgesia. J Clin Monit Comput 1998; 14 (4): 253-63
- White PF. Mishaps with patient-controlled analgesia. Anesthesiology 1987; 66 (1): 81-3
- Institute for Safe Medication Practices. Misprogram a PCA pump? It's easy! [online]. Available from URL: www.ismp. org/Newsletters/acutecare/articles/20040729_2.asp [Accessed 2008 May 15]
- Joint Commission on Accreditation of Healthcare Organizations. Patient controlled analgesia by proxy [online].
 Available from URL: http://www.jointcommission.org/ SentinelEvents/SentinelEventAlert/sea_33.htm [Accessed 2008 May 15]
- National Coordinating Council for Medication Error Reporting and Prevention. NCC MERP taxonomy of medication errors [online]. Available from URL: http://www.nccmerp.org/medErrorTaxonomy.html [Accessed 2008 May 15]
- Doyle DJ. Programming errors from patient-controlled analgesia. Can J Anaesth 2003; 50 (8): 855-6
- Kopp BJ, Erstad BL, Allen ME, et al. Medication errors and adverse drug events in an intensive care unit: direct observation approach for detection. Crit Care Med 2006; 34 (2): 415-25
- Rothschild JM, Landrigan CP, Cronin JW, et al. The Critical Care Safety Study: the incidence and nature of adverse events and serious medical errors in intensive care. Crit Care Med 2005; 33 (8): 1694-700
- Cina JL, Gandhi TK, Churchill W, et al. How many hospital pharmacy medication dispensing errors go undetected? Jt Comm J Qual Patient Saf 2006; 32 (2): 73-80
- Leape LL, Bates DW, Cullen DJ, et al. Systems analysis of adverse drug events. ADE Prevention Study Group. JAMA 1995; 274 (1): 35-43
- Ness JE, Sullivan SD, Stergachis A. Accuracy of technicians and pharmacists in identifying dispensing errors. Am J Hosp Pharm 1994; 51 (3): 354-7
- Rolland P. Occurrence of dispensing errors and efforts to reduce medication errors at the Central Arkansas Veteran's Healthcare System. Drug Saf 2004; 27 (4): 271-82

- Woller TW, Stuart J, Vrabel R, et al. Checking of unit dose cassettes by pharmacy technicians at three Minnesota hospitals. Am J Hosp Pharm 1991; 48 (9): 1952-6
- Youngs PJ. A problem with a PCA pump [letter]. Anaesthesia 1993; 48 (9): 829
- 62. White E. A problem with the Graseby 3300 PCA pump. Anaesthesia 1993; 48 (11): 1013-4
- Lin L, Vicente KJ, Doyle DJ. Patient safety, potential adverse drug events, and medical device design: a human factors engineering approach. J Biomed Inform 2001; 34 (4): 274-84
- Schug SA, Torrie JJ. Safety assessment of postoperative pain management by an acute pain service. Pain 1993; 55 (3): 387-91
- 65. Wakerlin G, Larson Jr CP. Spouse-controlled analgesia [letter]. Anesth Analg 1990; 70 (1): 119
- Johnson T, Daugherty M. Oversedation with patient controlled analgesia. Anaesthesia 1992; 47 (1): 81-2
- Bates DW, Vanderveen T, Seger D, et al. Variability in intravenous medication practices: implications for medication safety. Jt Comm J Qual Patient Saf 2005; 31 (4): 203-10
- Christie L, Cranfield KA. A dangerous fault with a PCA pump [letter]. Anaesthesia 1998; 53 (8): 827
- 69. Notcutt WG, Morgan RJ. Introducing patient-controlled analgesia for postoperative pain control into a district general hospital. Anaesthesia 1990; 45 (5): 401-6
- Notcutt WG, Knowles P, Kaldas R. Overdose of opioid from patient-controlled analgesia pumps. Br J Anaesth 1992; 69 (1): 95-7
- Thomas DW, Owen H. Patient-controlled analgesia: the need for caution. A case report and review of adverse incidents. Anaesthesia 1988; 43 (9): 770-2
- Doyle DJ, Vicente KJ. Electrical short circuit as a possible cause of death in patients on PCA machines: report on an opiate overdose and a possible preventive remedy [letter]. Anesthesiology 2001; 94 (5): 940
- Chan S, Chen PP, Chui PT, et al. Unintentional bolus with Graseby 9300 pump [letter]. Anaesth Intensive Care 1998; 26 (1): 117
- Doyle DJ, Nebbia SP. Intravenous dead space and patient safety in patient-controlled analgesia [letter]. Can J Anaesth 1995; 42 (7): 658
- Grey TC, Sweeney ES. Patient-controlled analgesia [letter]. JAMA 1988; 259 (15): 2240
- Sanchez-Guijo JJ, Benavente MA, Crespo A. Failure of a patient-controlled analgesia pump in a hyperbaric environment. Anesthesiology 1999; 91 (5): 1540-2
- Leeson-Payne CG, Towell T. Magnetic mayhem. Anaesthesia 1996; 51 (11): 1081-2
- Food and Drug Administration, Center for Devices and Radiological Health. Search MAUDE database [online]. Available from URL: http://www.accessdata.fda.gov/scripts/ cdrh/cfdocs/cfMAUDE/search.cfm [Accessed 2008 May 15]
- Hankin CS, Schein J, Clark JA, et al. Adverse events involving intravenous patient-controlled analgesia. Am J Health Syst Pharm 2007; 64 (14): 1492-9
- US Pharmacopeia. MEDMARX patient safety solutions. The National Database for Medication Errors [online]. Available from URL: https://www.medmarx.com/ [Accessed 2008 May 15]

- Santell JP, Cousins DD, Hicks R. Errors involving PCA pumps. Drug Topics 2004; Health-System Edition: 28-9
- Hicks RW, Sikirica V, Nelson W, et al. Medication errors involving patient-controlled analgesia. Am J Health Syst Pharm 2008; 65 (5): 429-40
- Rothschild JM, Keohane CA, Thompson S, et al. Intelligent intravenous infusion pumps to improve medication administration safety. AMIA Annu Symp Proc 2003; 992
- 84. Rothschild JM, Keohane CA, Cook EF, et al. A controlled trial of smart infusion pumps to improve medication safety in critically ill patients. Crit Care Med 2005; 33 (3): 533-40
- Wetterneck TB, Skibinski KA, Roberts TL, et al. Using failure mode and effects analysis to plan implementation of smart i.v. pump technology. Am J Health Syst Pharm 2006; 63 (16): 1528-38
- Rasmussen J. Information processing and human-machine interaction: an approach to cognitive engineering. New York: Elsevier Science Inc., 1986
- 87. Bates DW, Gawande AA. Improving safety with information technology. N Engl J Med 2003; 348 (25): 2526-34
- 88. Beers MH, Avorn J, Soumerai S, et al. Computer-assisted drug data collection. J Med Syst 1992; 16 (1): 1-6
- Kaushal R, Shojania KG, Bates DW. Effects of computerized physician order entry and clinical decision support systems on medication safety: a systematic review. Arch Intern Med 2003; 163 (12): 1409-16
- Kuperman GJ, Teich JM, Gandhi TK, et al. Patient safety and computerized medication ordering at Brigham and

- Women's Hospital. Jt Comm J Qual Improv 2001; 27 (10): 509-21
- Kuperman GJ, Gibson RF. Computer physician order entry: benefits, costs, and issues. Ann Intern Med 2003; 139 (1): 31-9
- Poon EG, Cina JL, Churchill W, et al. Medication dispensing errors and potential adverse drug events before and after implementing bar code technology in the pharmacy.
 Ann Intern Med 2006; 145 (6): 426-34
- Van de Castle B, Kim J, Pedreira ML, et al. Information technology and patient safety in nursing practice: an international perspective. Int J Med Inform 2004; 73 (7-8): 607-14
- Kuperman GJ, Gandhi TK, Bates DW. Effective drugallergy checking: methodological and operational issues.
 J Biomed Inform 2003; 36 (1-2): 70-9
- Oliven A, Zalman D, Shilankov Y, et al. Prevention of prescription errors by computerized, on-line, individual patient related surveillance of drug order entry. Stud Health Technol Inform 2002; 90: 632-4
- Paoletti RD, Suess TM, Lesko MG, et al. Using bar-code technology and medication observation methodology for safer medication administration. Am J Health Syst Pharm 2007; 64 (5): 536-43

Correspondence: Dr *Jeff R. Schein*, Ortho-McNeil Janssen Scientific Affairs, LLC, 1000 Route 202, Room 3202, Raritan, NJ 08869, USA.

E-mail: jschein@its.jnj.com