

## Short communication

## Indirect determination of pyruvic acid by capillary electrophoresis with amperometric detection

Xin Lu, Wei-Hua Huang <sup>\*</sup>, Feng Ai, Zong-Li Wang, Jie-Ke Cheng <sup>\*</sup>

*Department of Chemistry, Wuhan University, Wuhan, China*

Received 11 May 2007; accepted 25 July 2007

Available online 3 August 2007

### Abstract

A method of indirectly measuring pyruvic acid (PA) by capillary electrophoresis with amperometric detection is proposed for the first time. It is based on the oximation reaction between PA and hydroxylamine ( $\text{NH}_2\text{OH}$ ), and the quantification of PA was performed by direct and sensitive amperometric detection of excessive  $\text{NH}_2\text{OH}$  after the oximation reaction. This method displayed a good sensitivity, and the detection limits of  $\text{NH}_2\text{OH}$  and PA are  $1.76 \times 10^{-7}$  and  $3.88 \times 10^{-7}$  mol/L, respectively at  $\text{S}/\text{N} = 3$ . The linear relationship between the peak current and PA concentration is exhibited over the range from  $4 \times 10^{-6}$  to  $1 \times 10^{-4}$  mol/L. This method has been applied to determine PA in rat plasma with satisfactory results.

© 2007 Published by Elsevier B.V.

**Keywords:** Capillary electrophoresis; Amperometric detection; Carbon fiber microelectrode; Hydroxylamine; Pyruvic acid

### 1. Introduction

Pyruvate is an important chemical compound in biochemistry. It is the output of the metabolism of glucose known as glycolysis, and an intermediate compound in the metabolism of carbohydrates, proteins, and fats [1–3]. Exceptional change of pyruvic acid (PA) concentration in the body could influence health. The determination of PA can give valuable information as to the process of metabolism and reactions in clinic analysis and bioanalysis [4–6].

Capillary electrophoresis (CE) has become a powerful tool for rapid and automated analysis of complex mixtures in biological samples [7–10], but there were only a few reports on CE for PA detection. Simonet et al. [11] has measured pyruvate according to the absorptivity decrease based on the pyruvate/lactate dehydrogenase/β-NADH reaction systems. Yeung's group has indirectly determined lactate and pyruvate in single erythrocytes by capillary electrophoresis with fluorescence detection [12]. Compared with the optical detection, CE-amperometric detection (CE-AD) was proved to be a highly sensitive and sim-

ple method for most of electrochemical compounds [13–16], but pyruvate itself has no absolute redox peak appearing in its voltammograms at  $-0.2$ – $1.0$  V. An approach for electrochemical detection of PA was performed by using enzyme biosensors [17–19], but the instability and relative low anti-disturb performance of the biosensors confine their applications in real sample detections. Another approach for direct detection of PA has been achieved by oxidizing PA at a high potential, and the detection limit is  $8.0 \times 10^{-6}$  mol/L at 1.6 V [20]. But high current noise and unstable current resulted from high working potential would also restrict the detection sensitivity and selectivity.

The indirect electrochemical determination methods of PA can be developed based on detecting the electroactive reactants or products associated with the PA chemical reactions. By oximation reaction that has been widely used to measure the content of carboxyl [21], PA can react with  $\text{NH}_2\text{OH}$  and forms oxime derivative, PA could be measured by detection of the electroactive compounds, hydroxylamine ( $\text{NH}_2\text{OH}$ ) or oxime derivative. Similar principle has been applied by Yu et al. to measuring p-tyrosine aminotransferase with HPLC-AD by detecting the oxime derivative [22]. However the approach of PA measurement based on  $\text{NH}_2\text{OH}$  detection has not been reported.

In this study, we have developed, for the first time, a method of indirect measuring PA based on the concentration change of  $\text{NH}_2\text{OH}$  which was sensitively and accurately detected by

<sup>\*</sup> Corresponding authors. Fax: +86 27 68754067.

E-mail addresses: [whuang@whu.edu.cn](mailto:whuang@whu.edu.cn) (W.-H. Huang), [jkcheng@whu.edu.cn](mailto:jkcheng@whu.edu.cn) (J.-K. Cheng).

CE-AD. There exists a perfectly linear relationship between the peak current and  $\text{NH}_2\text{OH}$  concentration ranged from  $4 \times 10^{-6}$  to  $1 \times 10^{-4}$  mol/L, and the detection limit is  $1.76 \times 10^{-7}$  mol/L. PA concentration has been investigated by monitoring the excessive  $\text{NH}_2\text{OH}$  concentration, this method exhibits a higher sensitivity and the detection limit of PA is  $3.88 \times 10^{-7}$  mol/L. The PA in rat plasma was measured by this method and the results showed good agreements with the value previously reported.

## 2. Materials and methods

### 2.1. Reagents and solutions

All chemicals were of analytical reagent grade and used as received without further purification. PA was prepared by dilution of 100 mM stock solution obtained by dissolving sodium pyruvate (biochemical reagent, Sinopharm group chemical reagent Co., Ltd., Shanghai, China) in 0.1 mol/L HCl. Hydroxylamine hydrochloride ( $\text{NH}_2\text{OH}\cdot\text{HCl}$ , analytical pure, Shanghai No. 4 reagent & H.V. chemical Co., Ltd. Shanghai, China) was prepared by dilution of 100 mM stock solution with the buffer solution. The standard solution of both PA and  $\text{NH}_2\text{OH}$  were daily prepared before using. All electrochemical and CE experiments were conducted in the pH 8.0 phosphate buffer saline (PBS) solution. All solutions were prepared with ultrapure water and sterilized by filtering through 0.2  $\mu\text{m}$  membrane filter units.

### 2.2. Apparatus

The laboratory-built capillary electrophoresis-electrochemical detection (CE-ED) system used for the experiments was similar to our group's previously described [23]. High voltage for the CE experiments was supplied by a +30 kV high voltage power source (Shanghai Institute of Nuclear Research, Shanghai, China), a fused-silica capillary (25  $\mu\text{m}$  i.d., 360  $\mu\text{m}$  o.d., length 65–70 cm, Yongnian Optical Fiber Factory, Hebei, China) was used throughout the CE experiments. The high voltage was applied in the injection end, while the reservoir containing electrochemical detection system was held at ground potential.

The end-column amperometric detection was performed by a two-electrode configuration. A carbon fiber microelectrode (CFME) with diameter of 8  $\mu\text{m}$  and exposed length of 100–200  $\mu\text{m}$ , which was prepared as described previously [24], was employed as the working electrode, a SCE and Ag/AgCl electrode worked as reference electrode in end-column amperometric detection and cyclic voltammetry, respectively. The working electrode was inserted into the end capillary about 5  $\mu\text{m}$  deep with the aid of a micromanipulator. All electrochemical detections were performed with a CHI660A electrochemical workstation (CH Instruments, Shanghai, China) in conjunction with a computer. The system was enclosed in a copper mesh Faraday cage to minimize the external noise.

### 2.3. Sample preparation

1 mL blood sampled from a rat that had not been fed for 8 h was then put into a 1 mL centrifugal tube before adding 15  $\mu\text{L}$

4% EDTA anticoagulate. Shake it to well distribution, quickly cool it in ice water (0 °C) for 15 min, and spin in a centrifuge at 2000 rpm for 15 min, supernatant liquid (the plasma) was collected into another centrifugal tube and stored in the refrigerator at –18 °C. The plasma was put into ice water prior to being added in the  $\text{NH}_2\text{OH}$  solution for oximation reaction.


### 2.4. Electrophoresis method

New separation capillary was treated with 0.1 mol/L NaOH, 0.1 mol/L HCl and doubly distilled water in sequence prior to use and balanced with electrophoresis buffer overnight, the capillary was washed with buffer during every run. Injection was performed electrokinetically at 15 kV for 8 s; separations were carried out at an applied voltage of 15 kV.

## 3. Results and discussions

### 3.1. Reaction mechanism

PA ( $\text{CH}_3\text{COCO}_2\text{H}$ ) is an alpha-keto acid and its carboxylate anion is known as pyruvate. PA can form the oxime derivative as the reaction scheme below:

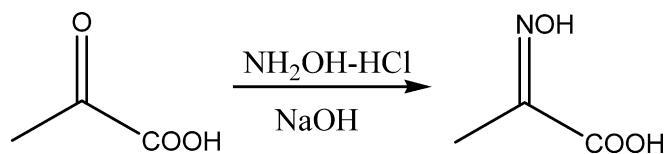

From the chemical equation above, PA can react with  $\text{NH}_2\text{OH}$ , a compound that can be directly electrochemically detected, to form oxime as the product. The PA could be quantified by CE separation followed by amperometric detection of the excessive  $\text{NH}_2\text{OH}$ , and the indirect methods of measuring PA could therefore be developed.

### 3.2. Detection of $\text{NH}_2\text{OH}$

#### 3.2.1. Detection potential of $\text{NH}_2\text{OH}$

Detection of  $\text{NH}_2\text{OH}$  is very important, since  $\text{NH}_2\text{OH}$  is not only the key reactant but also the final detected reagent in the whole process of this method. No obvious oxidation peak at carbon fiber microelectrode (CFME) was observed from the cyclic voltammetry of  $\text{NH}_2\text{OH}$  in the potential range from –0.20 to +1.60 V (Fig. 1). The current shows an increase caused by the  $\text{NH}_2\text{OH}$  oxidation on the CFME when the applied potential above 0.30 V, and the oxidation current increases rapidly with the positive shift of applied potential from 0.60 V, until the sharp rising of the current from the oxygen evolution when the potential is over 1.40 V. The electrophoresis peak current of  $\text{NH}_2\text{OH}$  at different working potential ranging from 0.60 to 1.40 V were investigated and the optimum detection performance was obtained at the voltage of 1.2 V with a compromise between high sensitivity and low background current.

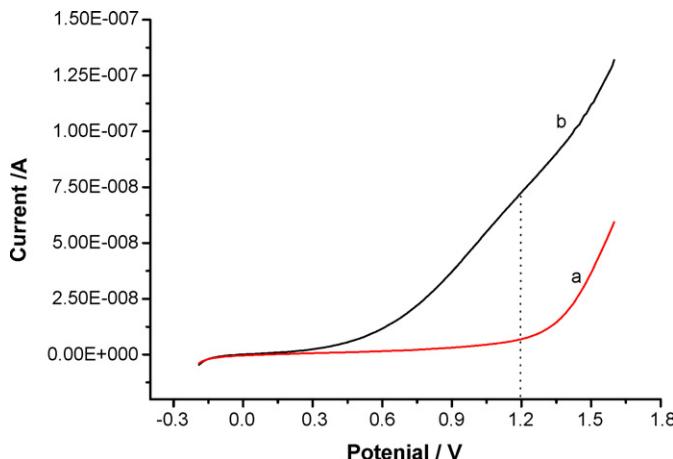


Fig. 1. Cyclic voltammograms (only positive scan represented here) at a CFME in the absence of NH<sub>2</sub>OH (a) and in the presence of 1 × 10<sup>-4</sup> mol/L NH<sub>2</sub>OH (b). The cyclic voltammetry scan was done in the range of -0.2 to 1.6 V with scan rate of 100 mV/s in phosphate buffer (pH 8.0), potential vs. Ag/AgCl.

### 3.2.2. Optimization of the separation and detection conditions

It was reported that the electrochemical behaviors of NH<sub>2</sub>OH was influenced by electrolyte pH [25]. The effect of electrolyte pH on the electrochemical as well as CE-AD behaviors of NH<sub>2</sub>OH was investigated, and the results showed that the maximum oxidation current (Fig. 2) and best separation performance of NH<sub>2</sub>OH was obtained at pH 8.00. Therefore a 10 mmol/L phosphate solution (pH 8.00) was used as the buffer in both the electrochemical and CE-AD experiments. The separation voltage and injection time for CE detection were also optimized as 15 kV and 8 s at 15 kV respectively.

### 3.2.3. Detection limit and linear range of NH<sub>2</sub>OH

Since the indirect methods of measuring PA is based on the direct monitoring the NH<sub>2</sub>OH concentration, the CE-AD performance of NH<sub>2</sub>OH plays important roles for the indirect measuring method. The CE-AD results showed that NH<sub>2</sub>OH could be determined by CE-AD with high sensitivity (Fig. 3),

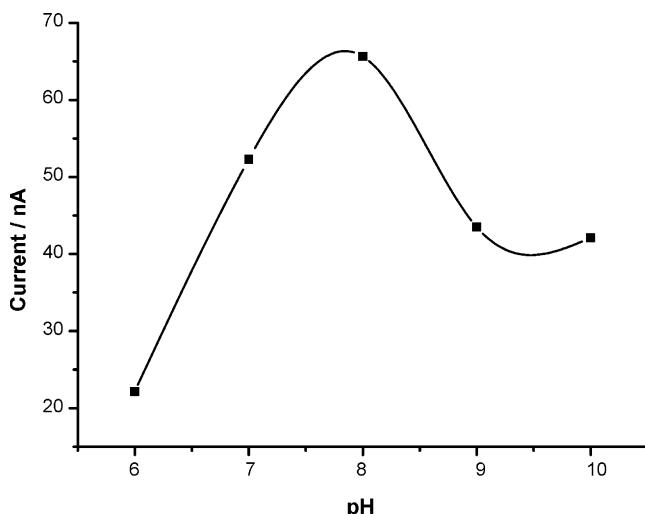


Fig. 2. The effect of pH on oxidation current of 1 × 10<sup>-3</sup> mol/L NH<sub>2</sub>OH.

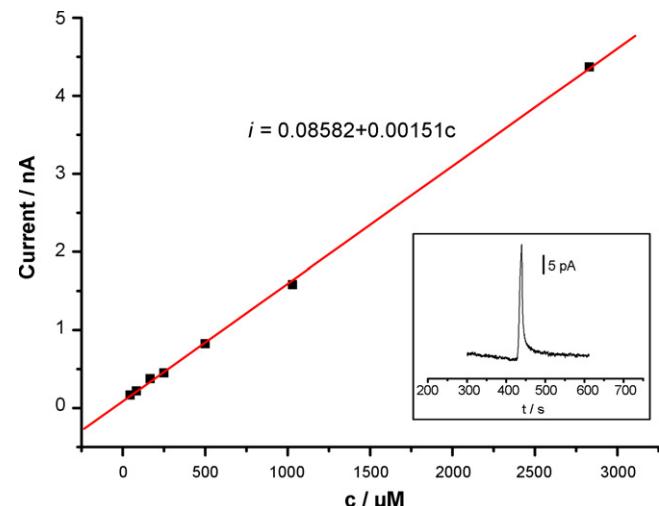


Fig. 3. Linear relationship between the peak current and concentration of NH<sub>2</sub>OH and the electropherogram of 1.2 × 10<sup>-6</sup> mol/L NH<sub>2</sub>OH (insert). Conditions: electrophoresis buffer, 10 mmol/L PBS at pH 8.0; separation voltage, 15 kV; injection time, 8 s; detection potential, 1.2 V.

the linear relationship between NH<sub>2</sub>OH peak current and its concentration was investigated at optimum experimental conditions. The results demonstrated that excellent linearity was obtained over the concentration range from 1.2 × 10<sup>-6</sup> to 1 × 10<sup>-2</sup> mol/L with a correlation coefficient ( $R^2$ ) of 0.9996. The detection limit of NH<sub>2</sub>OH was 1.76 × 10<sup>-7</sup> mol/L (S/N = 3).

### 3.3. Indirect measurement of PA

This study aimed at the investigation of PA concentration by CE-AD, which is developed on the quantitative reaction between PA and NH<sub>2</sub>OH, and subsequent detection of NH<sub>2</sub>OH. The quantitative information of the PA could herewith be obtained by detecting the NH<sub>2</sub>OH before and after the oximation reaction.

#### 3.3.1. Optimization of the reaction conditions between PA and NH<sub>2</sub>OH

It was demonstrated that the reaction between PA and free NH<sub>2</sub>OH is a quick and complete process [21], and the indirect method was herewith established. The reaction conditions such as reaction time, temperature, etc. have been optimized for setting up a fast and quantitative equilibrium. Heating will accelerate the reaction, but high temperature would also result in the instability of NH<sub>2</sub>OH. The reaction temperature and reaction time were finally optimized at 50 °C and 5 min, respectively, under such conditions a complete reaction and optimum CE-AD performance could be achieved, and PA concentration has a good linear relationship with the consumed NH<sub>2</sub>OH.

#### 3.3.2. Quantification of PA

According to the principle of the indirect measurement method, the quantification of PA was obtained by peak current decrease of NH<sub>2</sub>OH from CE-AD detection caused by the oximation reaction between PA and NH<sub>2</sub>OH. The original NH<sub>2</sub>OH concentration before reaction was constant as about 10-folds higher than PA for a compromise between a complete reaction

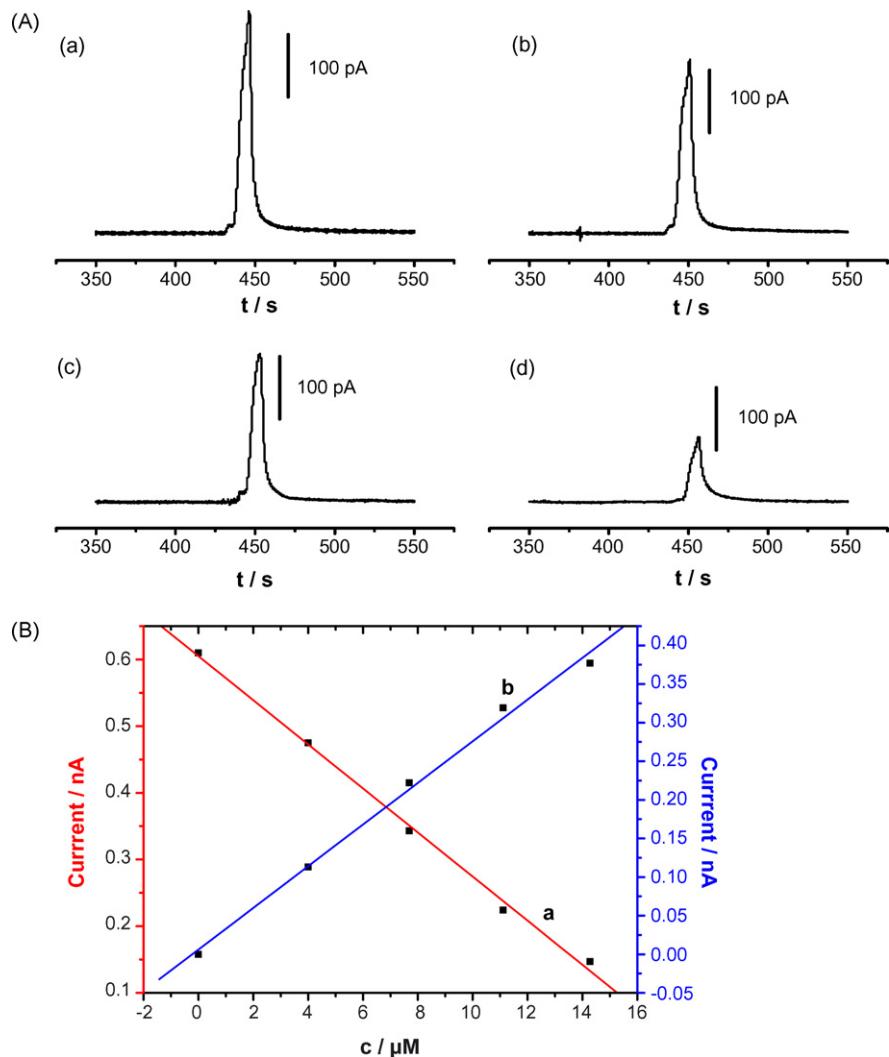


Fig. 4. (A) Electropherogram of  $1 \times 10^{-4}$  mol/L  $\text{NH}_2\text{OH}$  reacted with (a) 0; (b) 4.0; (c) 7.7; (d) 14.2  $\mu\text{mol/L}$  PA. (B) Linear relationship between the peak current of  $\text{NH}_2\text{OH}$  (a) or peak current decreases caused by the  $\text{NH}_2\text{OH}$  consumption during oximation reaction (b) and the PA concentration.

and high sensitivity. Fig. 4A described the electropherograms of excessive  $\text{NH}_2\text{OH}$  after oximation reaction with different amount of PA. The peak currents ( $i$ ) of  $\text{NH}_2\text{OH}$  showed a good linear relationship with the concentration of added PA

(Fig. 4B, a) which was further deduced as the linear relationship between the peak current decreases ( $i_{\text{decr}}$ ) caused by the  $\text{NH}_2\text{OH}$  consumption during oximation reaction and PA concentration (Fig. 4B, b). The results demonstrated that both  $i$  and  $i_{\text{decr}}$  are in good linear dependence with the PA concentration in the range from  $4 \times 10^{-6}$  to  $1 \times 10^{-4}$  mol/L. The linear response are given by the equation  $i = 0.6051 - 0.03307c$  ( $R^2 = 0.9966$ ) and  $i_{\text{decr}} = 0.00606 + 0.02699c$  ( $R^2 = 0.9948$ ), respectively, where  $i$  and  $i_{\text{decr}}$  are the amperometric response in nA and  $c$  is the PA concentration in  $\mu\text{M}$ . The detection limit of PA was  $3.88 \times 10^{-7}$  ( $S/N = 3$ ), which is lower than previously reported [20] and thus facilitates the detection of trace amount of PA in bioanalysis and clinical analysis.

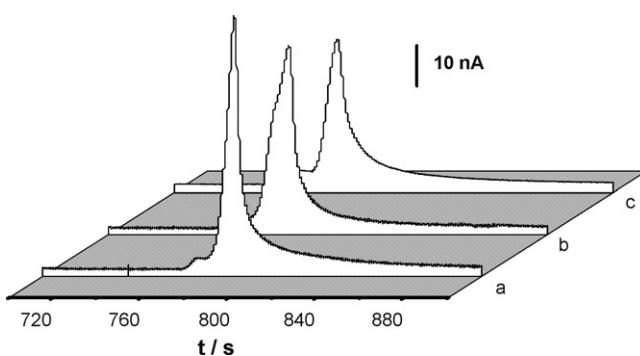


Fig. 5. The electropherograms of  $1 \times 10^{-4}$  mol/L  $\text{NH}_2\text{OH}$  (a),  $1 \times 10^{-4}$  mol/L  $\text{NH}_2\text{OH}$  after being reacted with  $1 \times 10^{-5}$  mol/L PA (b) and  $1 \times 10^{-4}$  mol/L  $\text{NH}_2\text{OH}$  after being reacted with plasma sample (c, the plasma sample was diluted 12.8 times before reaction) PA in PBS at pH8.0, the other conditions used were the same as described in Fig. 3.

### 3.4. Measurement of PA in plasma

The kinetic change of PA concentration indicates the intensity of metabolism. The normal concentration of PA is between  $8.74 \times 10^{-5}$  and  $1.96 \times 10^{-4}$  mol/L. The PA concentration is an important index for pathological diagnosis and abnor-

mal increase or decrease of PA concentration will also cause metabolism related diseases such as pyruvate acidosis. We have applied this indirect method to determine PA concentration in rat plasma. The electropherogram of  $\text{NH}_2\text{OH}$  in PBS at pH 8.0 was showed as (a) in **Fig. 5**, and (b and c) illustrate the electropherograms of  $\text{NH}_2\text{OH}$  followed by reaction with  $1 \times 10^{-5}$  mol/L standard PA and with the rat plasma sample, respectively. The experiment data was analyzed and the PA concentration in rat plasma was found to be  $1.43 \pm 0.45 \times 10^{-4}$  mol/L ( $n=6$ ), which is in good agreement with the value reported before.

#### 4. Conclusion

In this paper, an indirect determining method of PA by CE-AD is proposed for the first time. Oximation between PA and  $\text{NH}_2\text{OH}$  followed by CE-AD of excessive  $\text{NH}_2\text{OH}$  made it a sensitive technique for PA determination. The linear relationship between the peak current and PA concentration was found in the range from  $4 \times 10^{-6}$  to  $1 \times 10^{-4}$  mol/L, and the detection limit of PA was  $3.88 \times 10^{-7}$  mol/L at  $\text{S}/\text{N}=3$ . The method has been successfully applied to investigate PA in rat plasma. This method is simple, sensitive, and easy to generalize, and would find its potential application in biological and clinical analysis.

#### Acknowledgements

This work was supported by the National Natural Science Foundation of China (Nos. 20405012, 20575056 and 20675060).

#### References

- [1] Y.H. Ko, B.L. Smith, Y. Wang, M.G. Pomper, D.A. Rini, M.S. Torbenson, J. Hullihen, P.L. Pedersen, *Biochem. Biophys. Res. Commun.* 324 (2004) 269.
- [2] T.K.T. Lam, R. Gutierrez-Juarez, A. Pocai, L. Rossetti, *Science* 209 (2005) 943.
- [3] H. Okada, S. Araga, T. Takshima, K. Nakashima, *Headache* 38 (1998) 39.
- [4] H. Krasinska-Czerlunczakiewicz, M. Pilarczyk, Z. Stelmasiak, *Neurol. Neurochir. Pol.* 32 (1999) 113.
- [5] T. Sommer, J.F. Larsen, *Brit. J. Surg.* 91 (2004) 855.
- [6] F.C. Cheng, D.Y. Yang, T.F. Wu, S.H. Chen, *J. Chromatogr. B* 723 (1999) 31.
- [7] S. Zhou, *J. Chromatogr. B* 797 (2003) 63.
- [8] Z. Glatz, *J. Chromatogr. B* 841 (2006) 23.
- [9] J. Kraly, Md.A. Fazal, R.M. Schoenher, R. Bonn, M.M. Harwood, E. Turner, M. Jones, N.J. Dovichi, *Anal. Chem.* 78 (2006) 4097.
- [10] R.J. Linhardt, T. Toida, *Science* 298 (2002) 1441.
- [11] B.M. Simonet, A. Rios, M. Valcarcel, *Electrophoresis* 25 (2004) 50.
- [12] Q. Xue, E.S. Yeung, *J. Chromatogr. A* 661 (1994) 287.
- [13] L.A. Holl, A.M. Leigh, *Electrophoresis* 23 (2002) 3649.
- [14] F.M. Matysik, *Electroanalysis* 17 (2000) 1349.
- [15] L.Y. Zhang, S.F. Qu, Z.L. Wang, J.K. Cheng, *J. Chromatogr. B* 792 (2003) 381.
- [16] Q. Weng, G. Xu, K. Yuan, P. Tang, *J. Chromatogr. B* 835 (2006) 55.
- [17] M.E. Ghica, C.M.A. Brett, *Electroanalysis* 18 (2006) 748.
- [18] M. Situmorang, J.J. Gooding, D.B. Hibbert, et al., *Electroanalysis* 14 (2002) 17.
- [19] A.F. Revzin, K. Sirkar, A. Simonian, M.V. Pishko, *Sens. Actuators B: Chem.* 81 (2002) 359.
- [20] M. Jin, Q. Dong, R. Dong, W. Jin, *Electrophoresis* 22 (2001) 2793.
- [21] Z.X. Zhang, R.G. Zhang, *Organic Functional Group quantitative analysis*, Chemical Industry Press, Beijing, China, 1990, p. 178.
- [22] P.H. Yu, B.A. Bailey, *J. Chromatogr.* 362 (1986) 55.
- [23] S. Hu, Z.L. Wang, P.B. Li, J.K. Cheng, *Anal. Chem.* 69 (1997) 264.
- [24] W.H. Huang, D.W. Pang, H. Tong, Z.L. Wang, J.K. Cheng, *Anal. Chem.* 73 (2001) 1048.
- [25] T. You, M. Wu, E. Wang, *Anal. Lett.* 30 (1997) 1025.